
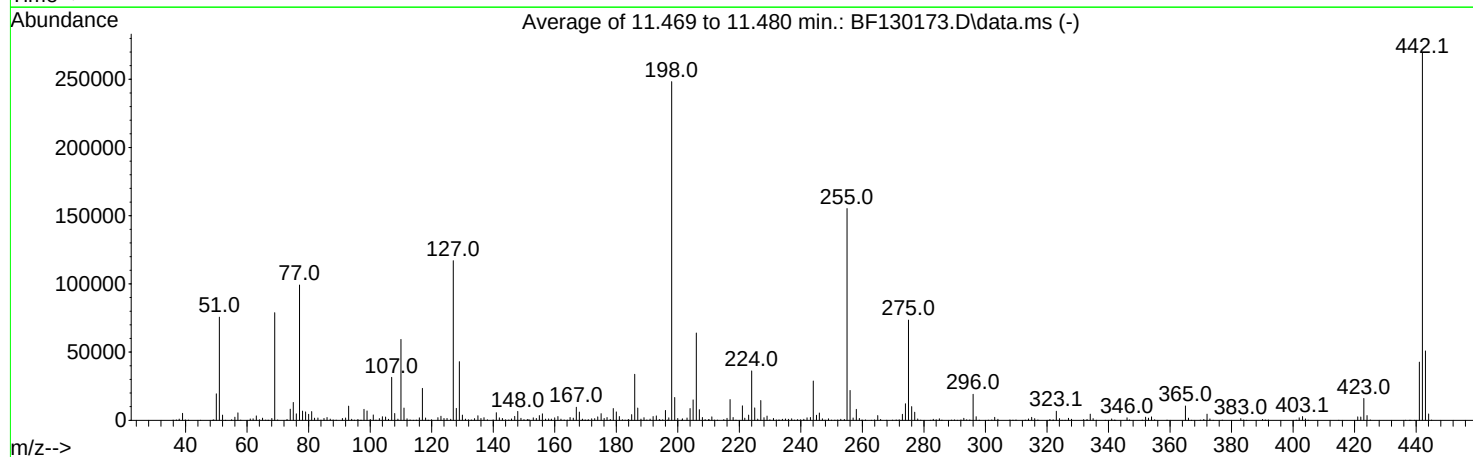


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090822\
 Data File : BF130173.D
 Acq On : 08 Sep 2022 09:37
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 07 02:05:07 2022

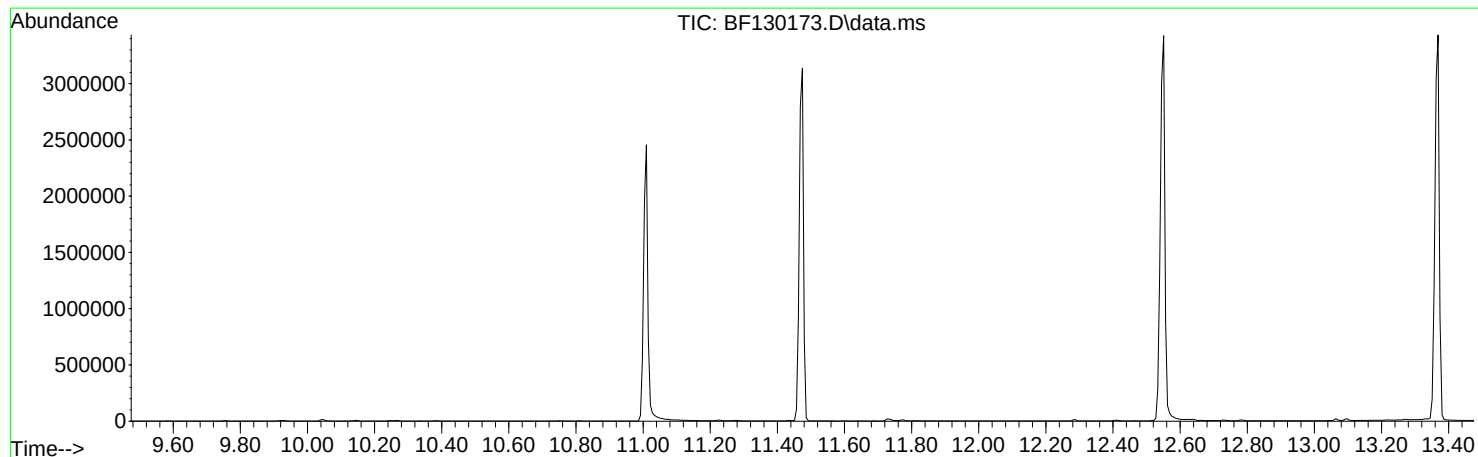




AutoFind: Scans 1561, 1562, 1563; Background Corrected with Scan 1555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	75649	PASS
68	69	0.00	2	1.7	1313	PASS
69	198	0.00	100	31.8	78851	PASS
70	69	0.00	2	0.4	353	PASS
127	198	10	80	47.1	117000	PASS
197	198	0.00	2	0.7	1789	PASS
198	198	100	100	100.0	248299	PASS
199	198	5	9	6.7	16726	PASS
275	198	10	60	29.6	73531	PASS
365	198	1	100	4.2	10476	PASS
441	198	0.01	100	17.2	42621	PASS
442	442	50	100	100.0	269696	PASS
443	442	15	24	18.9	50893	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090822\
Data File : BF130173.D
Acq On : 08 Sep 2022 09:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 09 06:10:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 07 02:05:07 2022
Response via : Initial Calibration

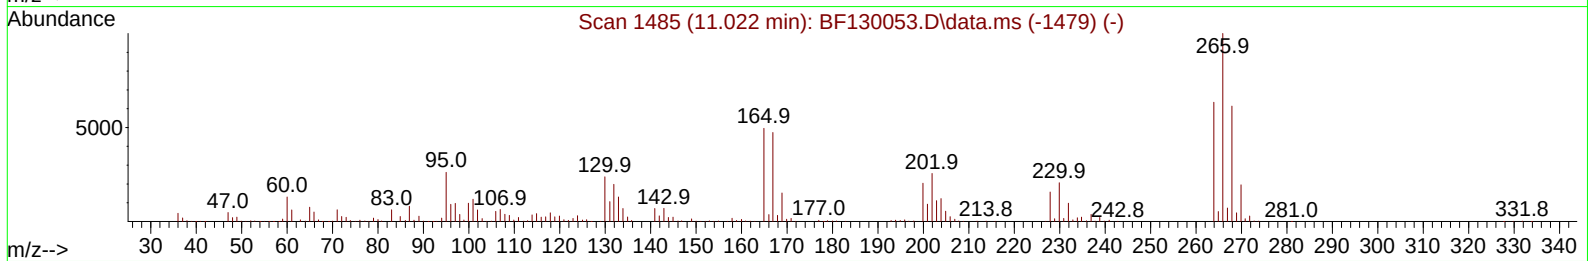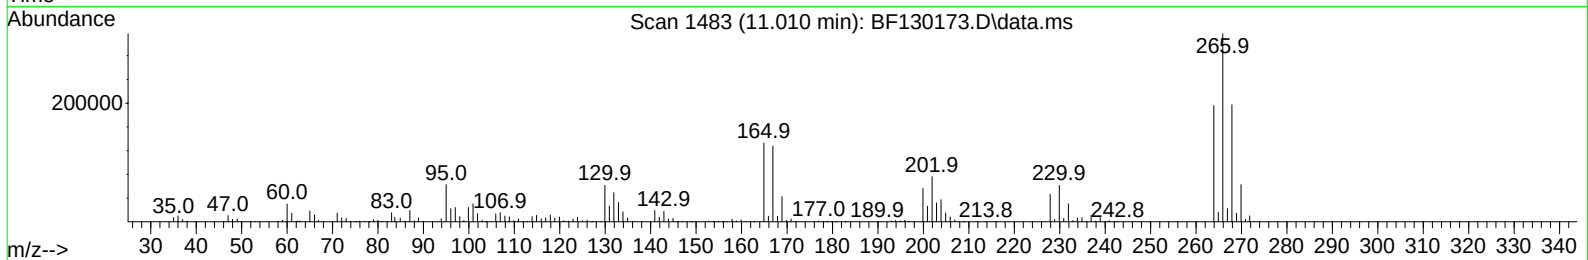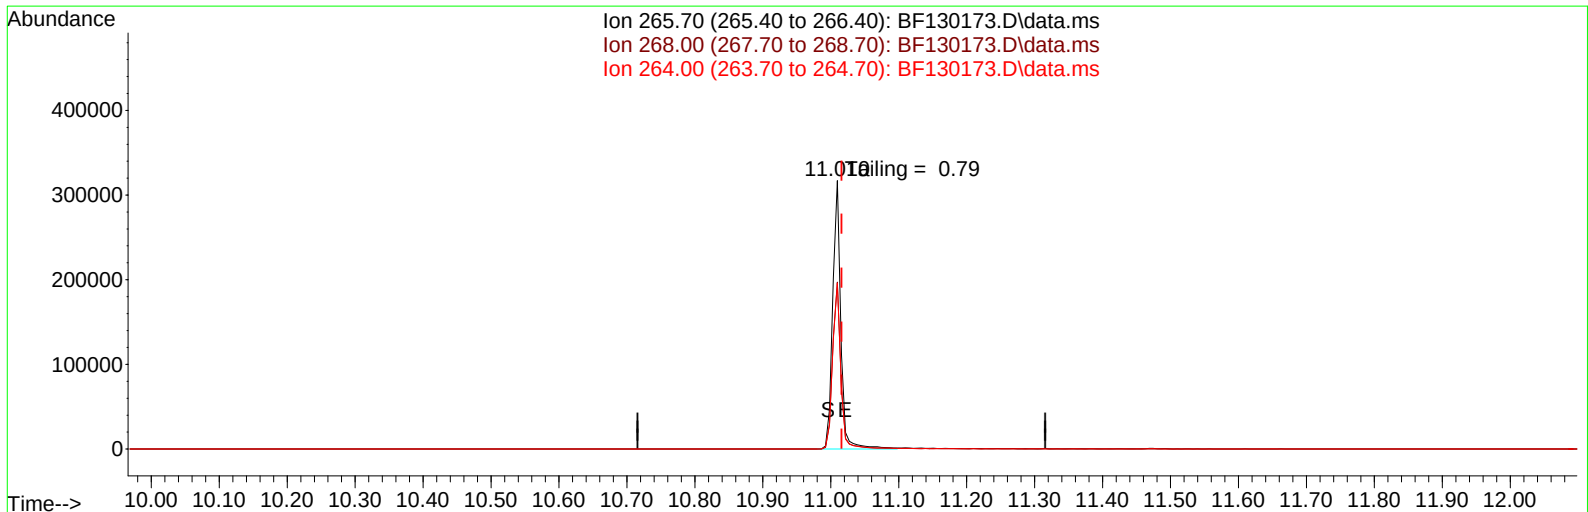

TIC: BF130173.D\data.ms

(70) Pentachlorophenol (C)

11.010min (-0.006) 209625.14 ng




response 262830

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.19
264.00	59.90	61.81
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090822\
Data File : BF130173.D
Acq On : 08 Sep 2022 09:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 09 06:10:52 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 07 02:05:07 2022
Response via : Initial Calibration

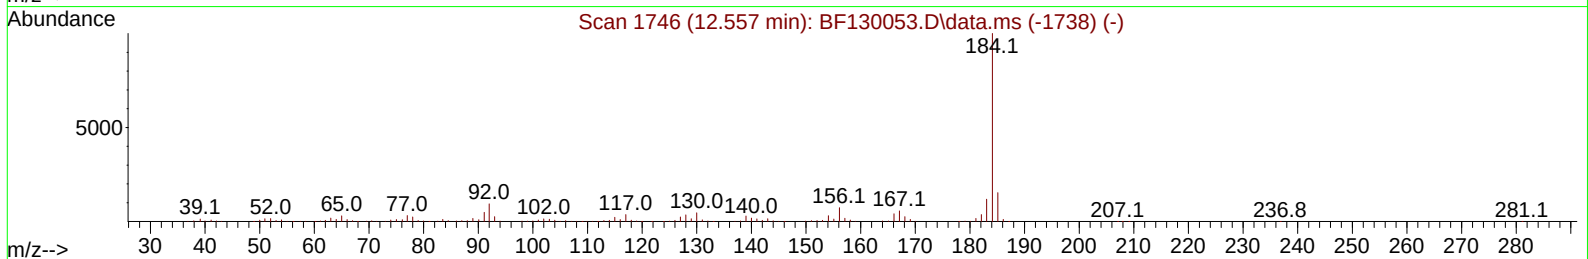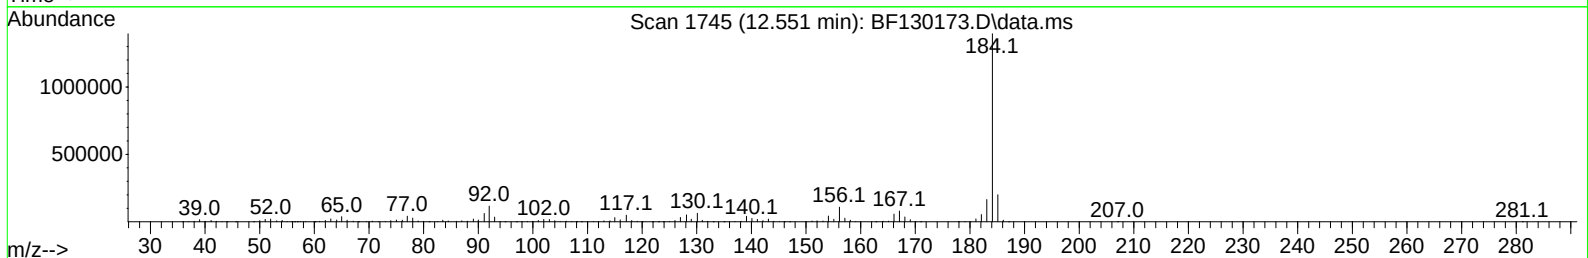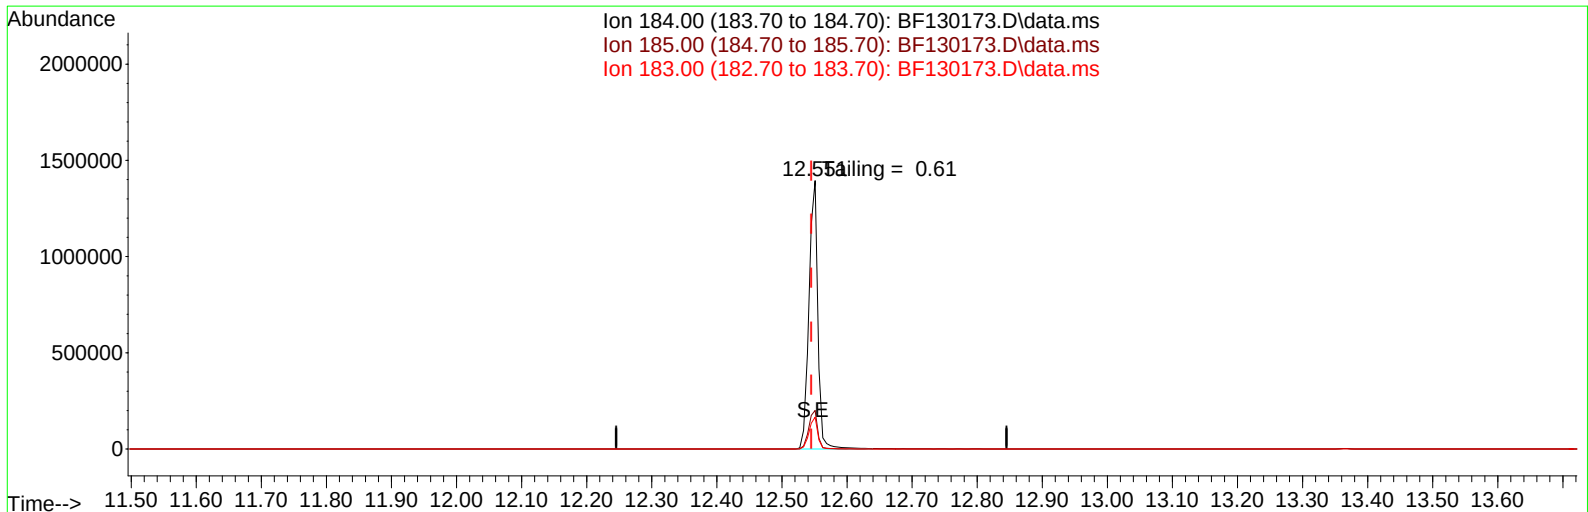

TIC: BF130173.D\data.ms

(77) Benzidine

12.551min (+ 0.006) 209831.06 ng

response 1331328

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	14.40
183.00	11.80	11.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/8/2022	BNA_F	<u>BF130173.D</u>
Compound Name	Response	Retention Time
DDT	585165	13.368
DDD	5326	13.063
DDE	1023	12.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6349	591514	1.07

Instrument :
BNA_F
ClientSampleId :
DFTPP