
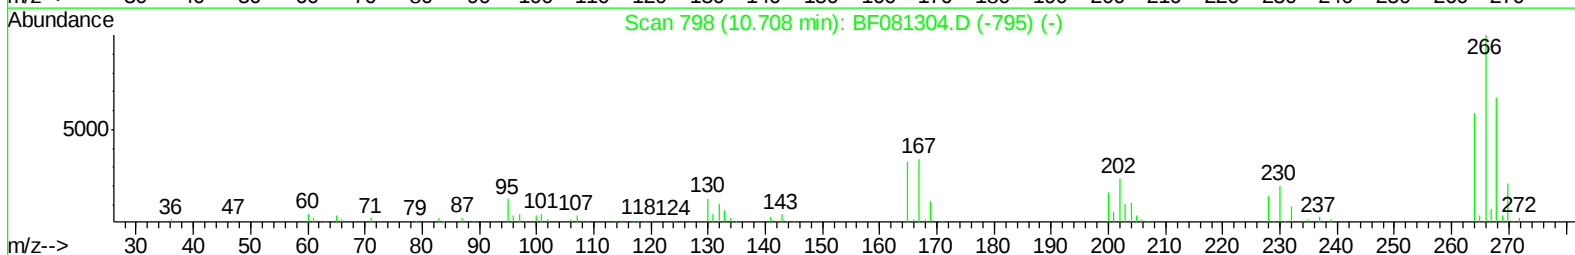
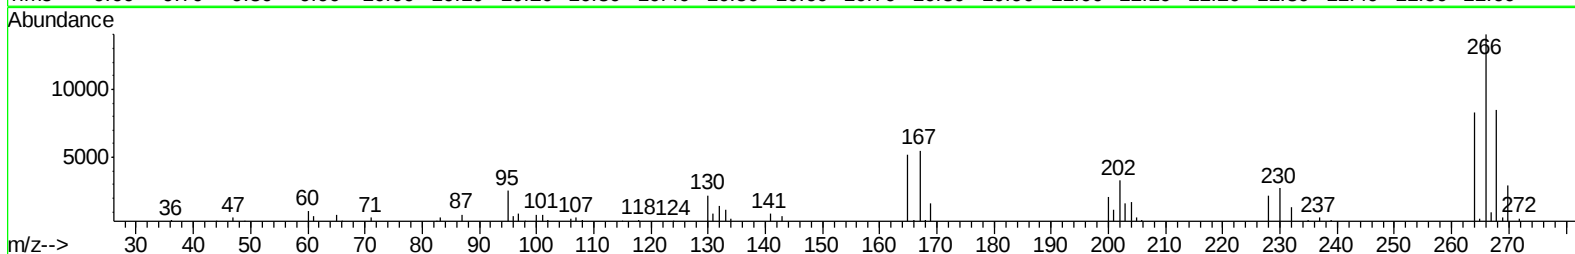


Data Path : Z:\HPCHEM1\BNA F\DATA\BF090915\
Data File : BF081554.D
Acq On : 9 Sep 2015 11:34
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 05:28:43 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 10 04:43:26 2015
Response via : Initial Calibration

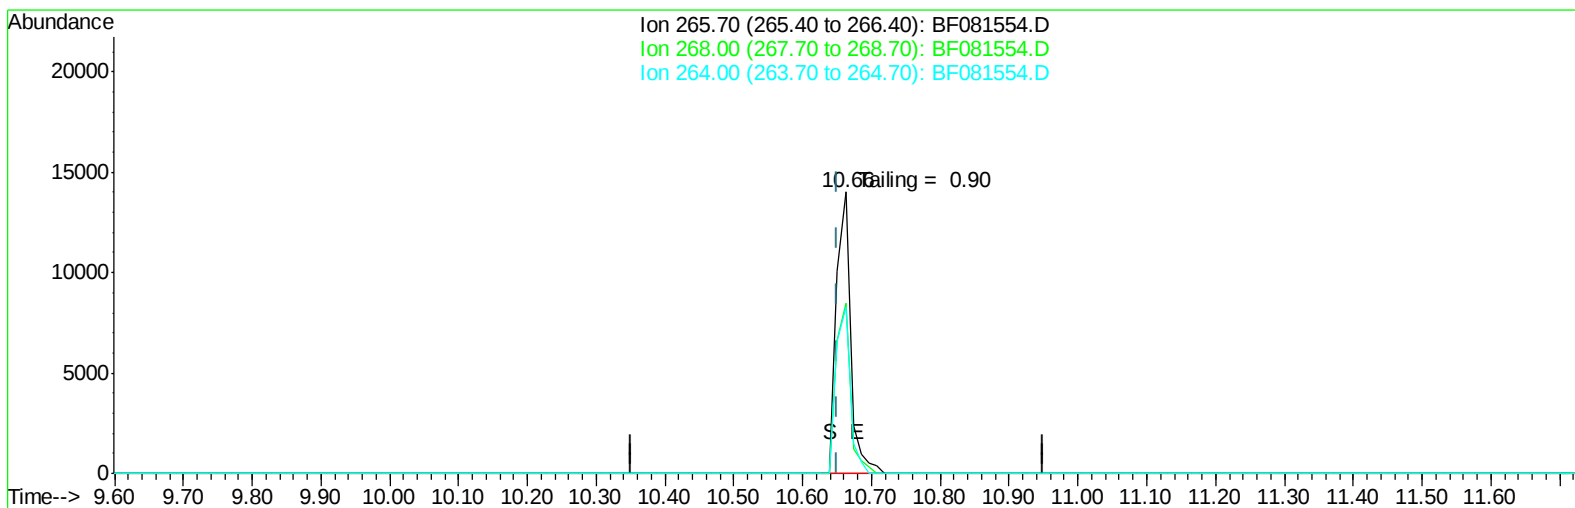

TIC: BF081554.D

(69) Pentachlorophenol (C)




10.662min (+0.011) 0.00ng

response 19405

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	60.27
264.00	62.70	59.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF090915\
Data File : BF081554.D
Acq On : 9 Sep 2015 11:34
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 05:28:43 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 10 04:43:26 2015
Response via : Initial Calibration

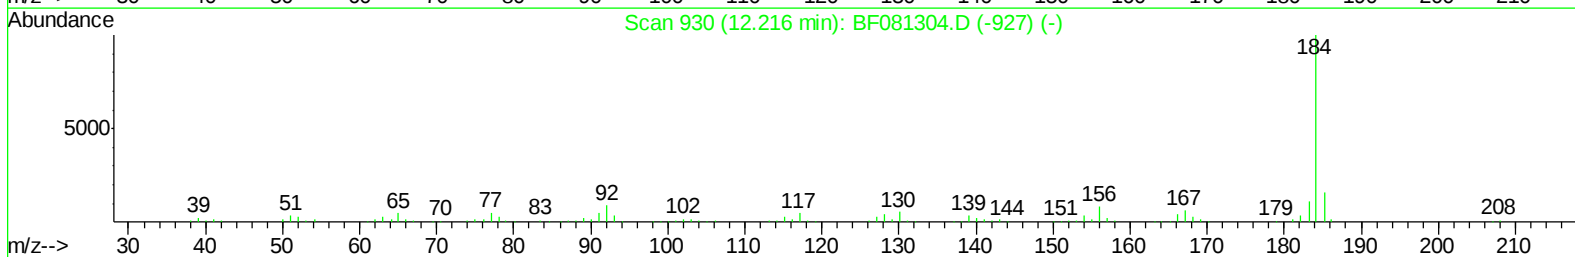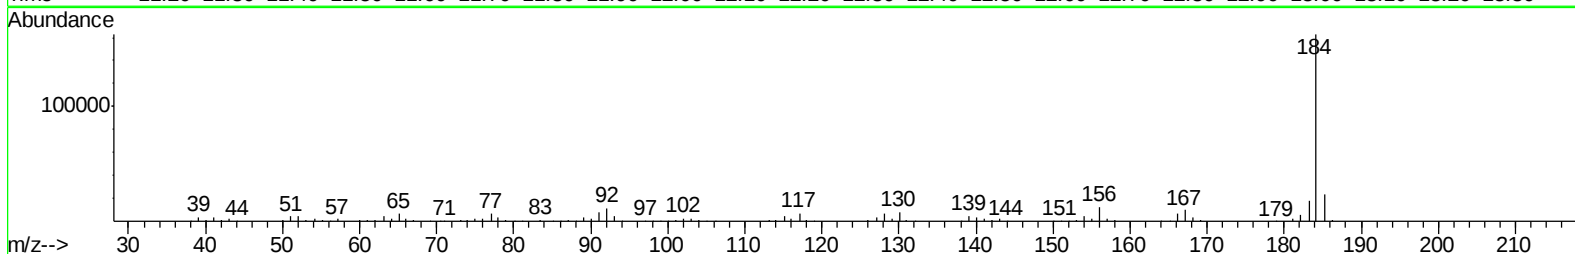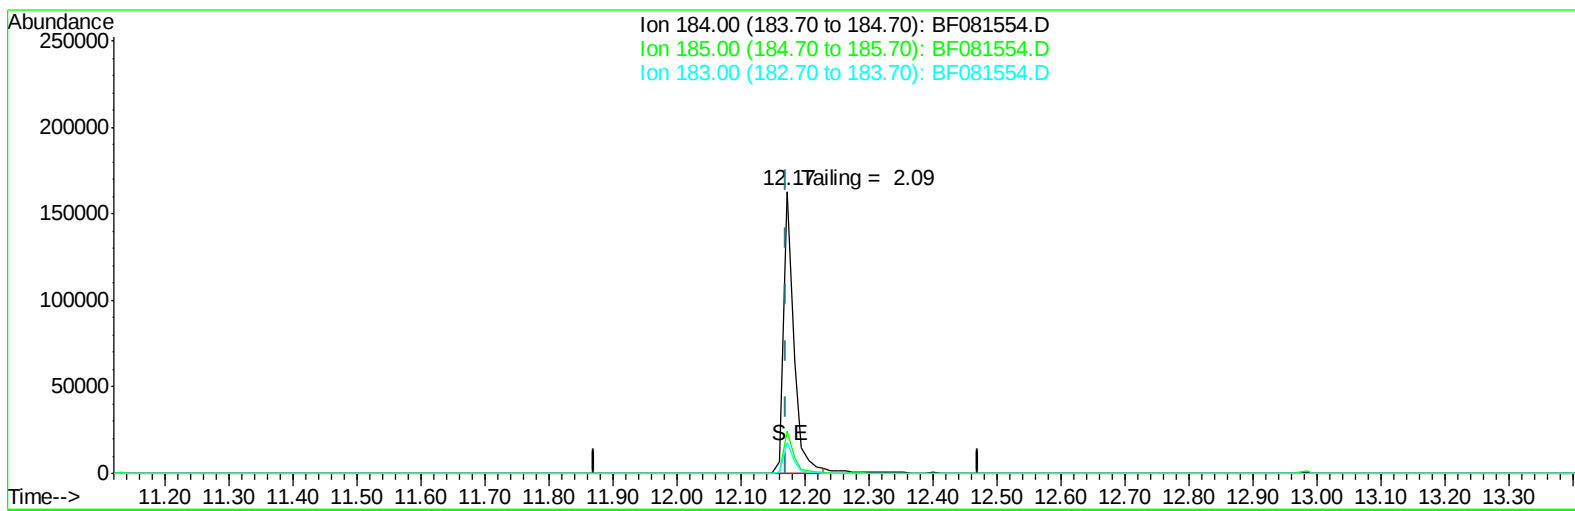

TIC: BF081554.D

(76) Benzidine

12.171min (-0.000) 0.00ng m

response 179857

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.82
183.00	9.50	11.02
0.00	0.00	0.00