


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090915\
Data File : BF081554.D
Acq On : 9 Sep 2015 11:34
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 10 04:35:20 2015

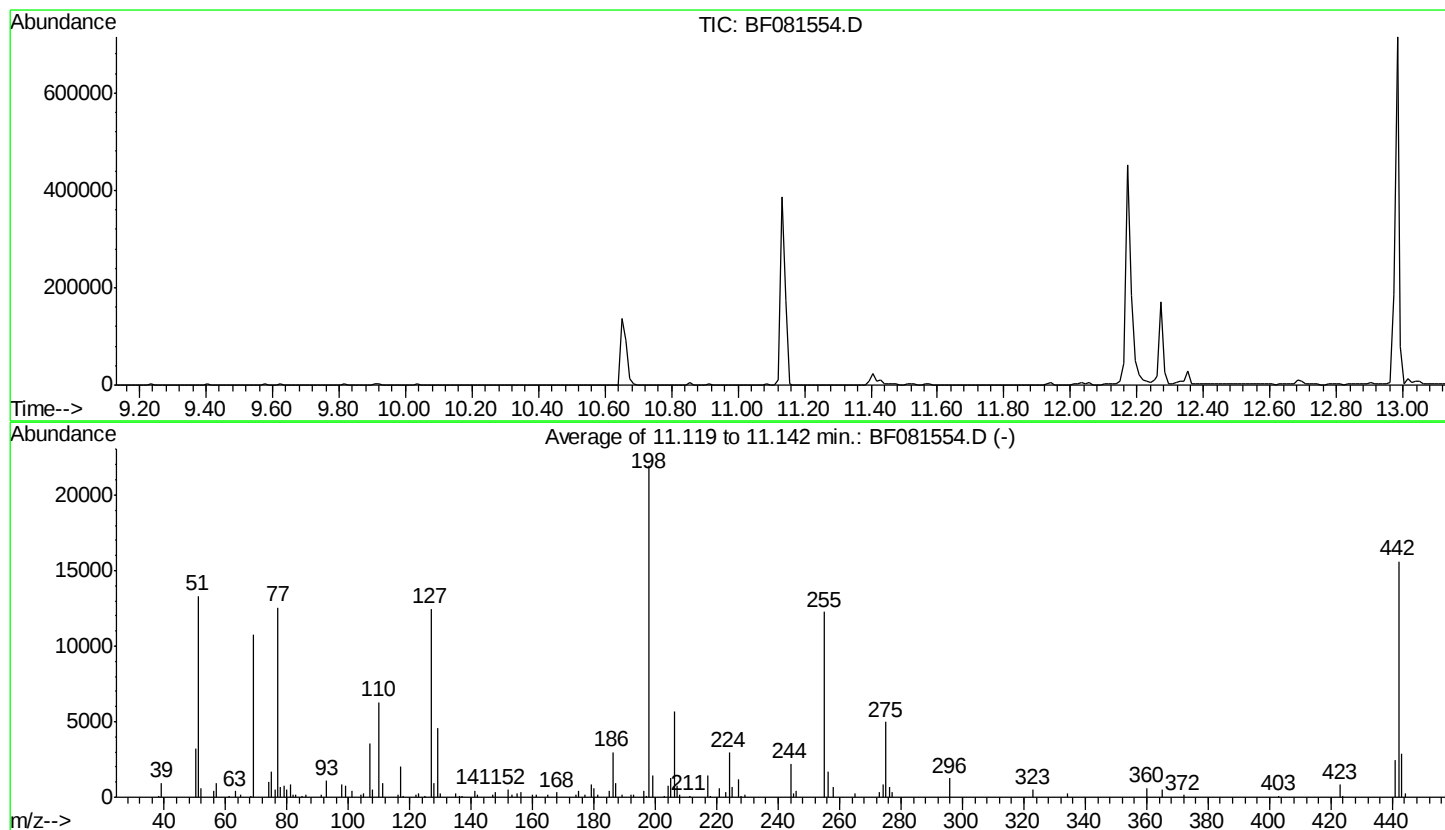

AutoFind: Scans 834, 835, 836; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.8	13343	PASS
68	69	0.00	2	1.0	110	PASS
69	198	0.00	100	49.1	10765	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.8	12466	PASS
197	198	0.00	2	0.5	105	PASS
198	198	100	100	100.0	21942	PASS
199	198	5	9	6.4	1409	PASS
275	198	10	60	22.7	4990	PASS
365	198	1	100	2.4	522	PASS
441	442	0.01	24	15.9	2488	PASS
442	198	50	100	71.1	15610	PASS
443	442	15	24	18.7	2913	PASS