
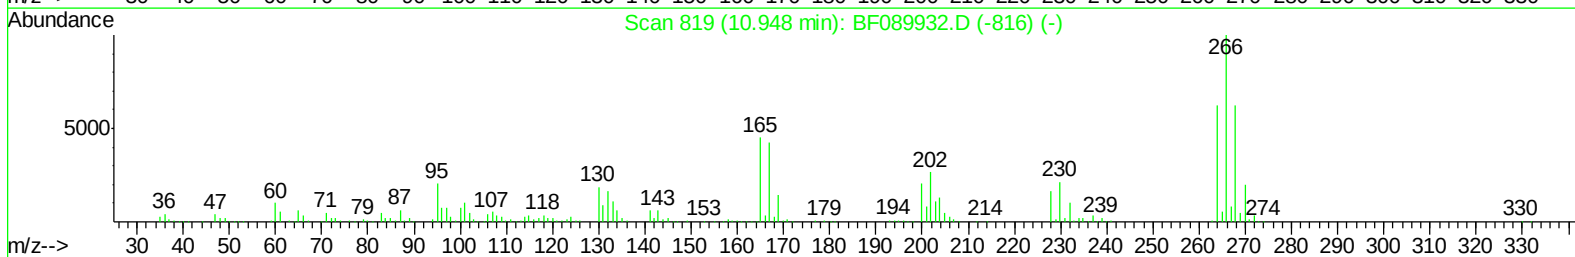
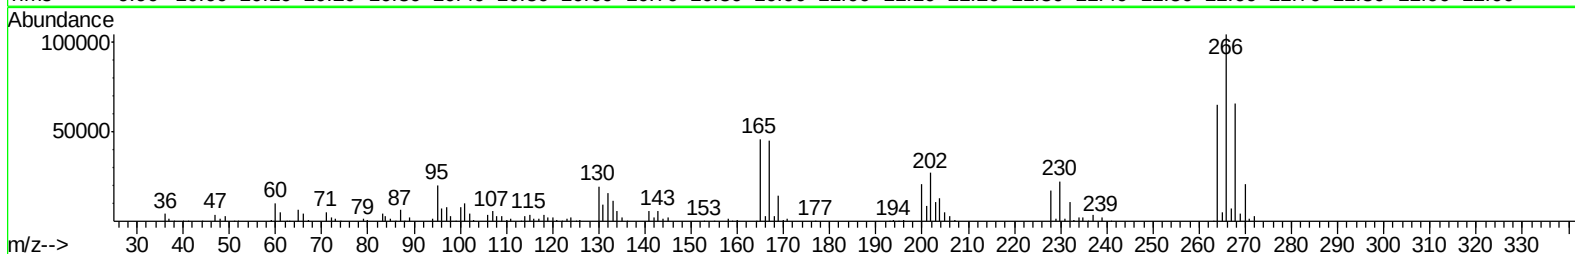


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090916\
Data File : BF090048.D
Acq On : 9 Sep 2016 13:45
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 06:41:30 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 08 16:07:52 2016
Response via : Initial Calibration

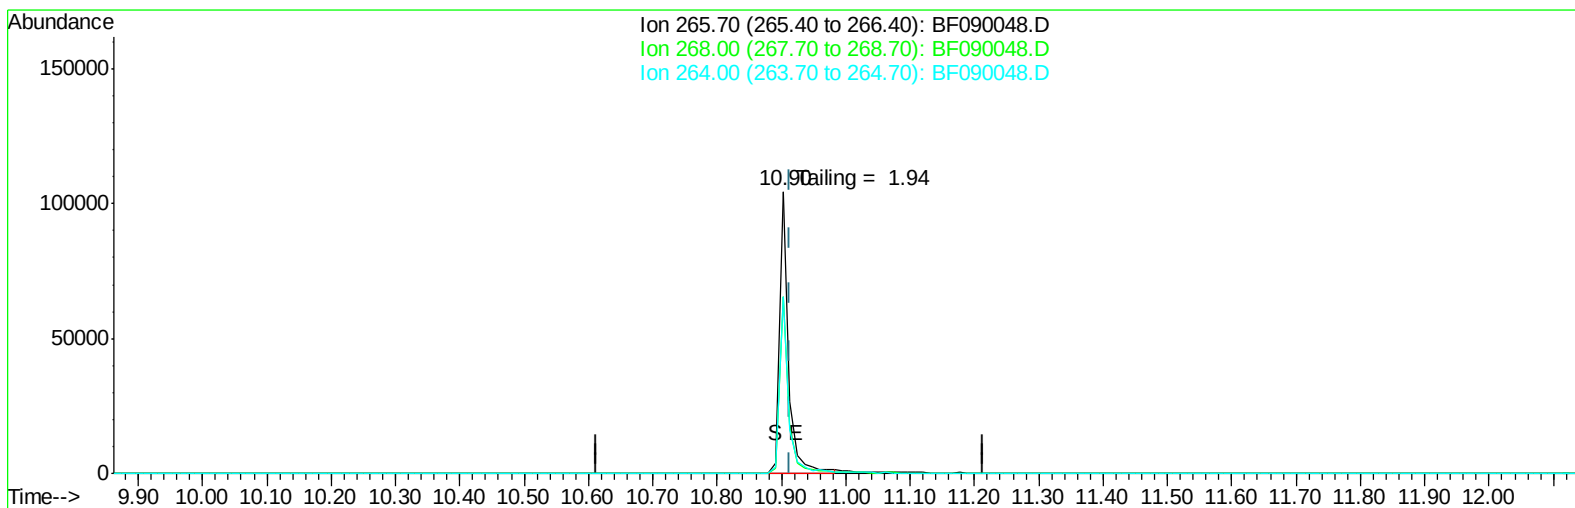

TIC: BF090048.D

(69) Pentachlorophenol (C)




10.902min (-0.011) 0.00ng

response 108028

Ion	Exp%	Act%
265.70	100	100
268.00	63.80	62.93
264.00	63.20	62.57
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090916\
Data File : BF090048.D
Acq On : 9 Sep 2016 13:45
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 06:41:30 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 08 16:07:52 2016
Response via : Initial Calibration

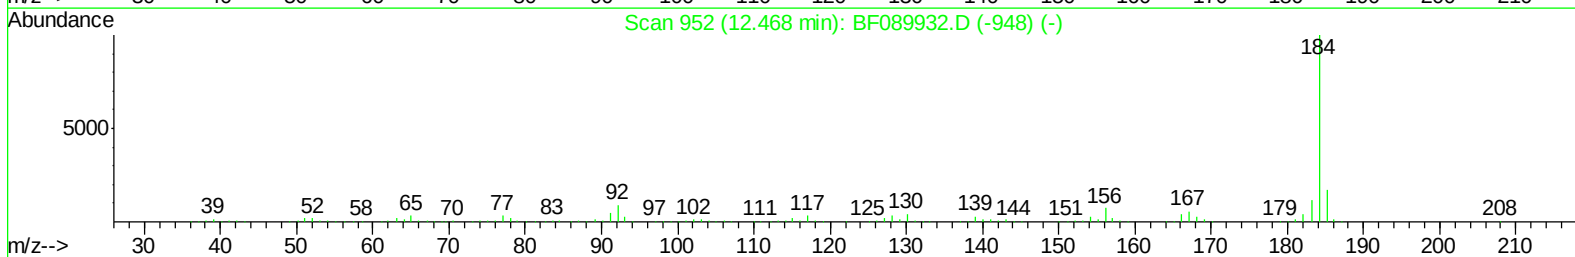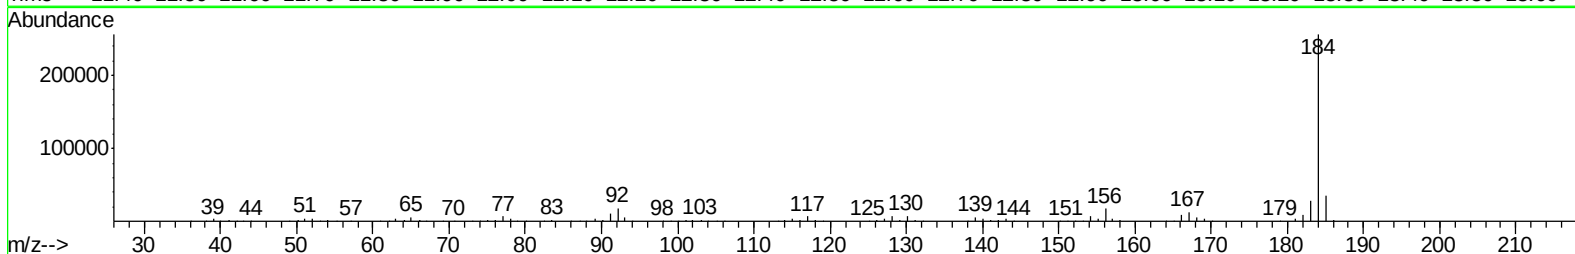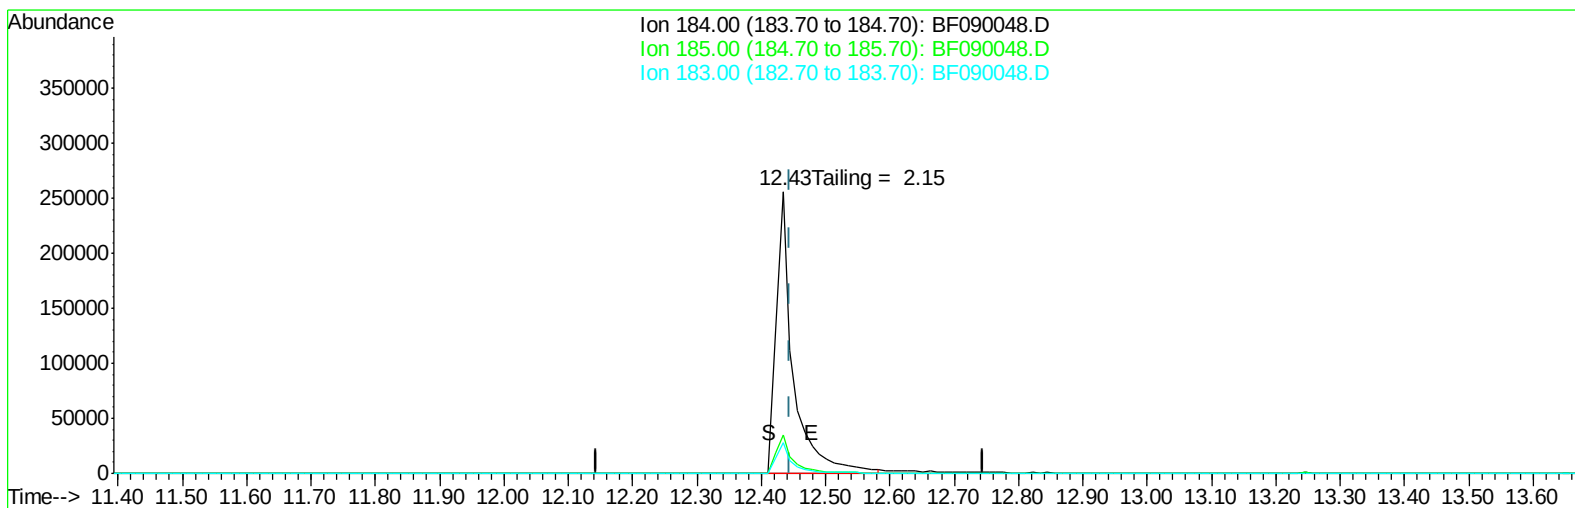

TIC: BF090048.D

(76) Benzidine

12.434min (-0.011) 11204.13ng

response 483021

Ion	Exp%	Act%
184.00	100	100
185.00	17.30	13.63#
183.00	12.00	10.77
0.00	0.00	0.00