


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF090916\
 Data File : BF090048.D
 Acq On : 9 Sep 2016 13:45
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 08 16:07:52 2016

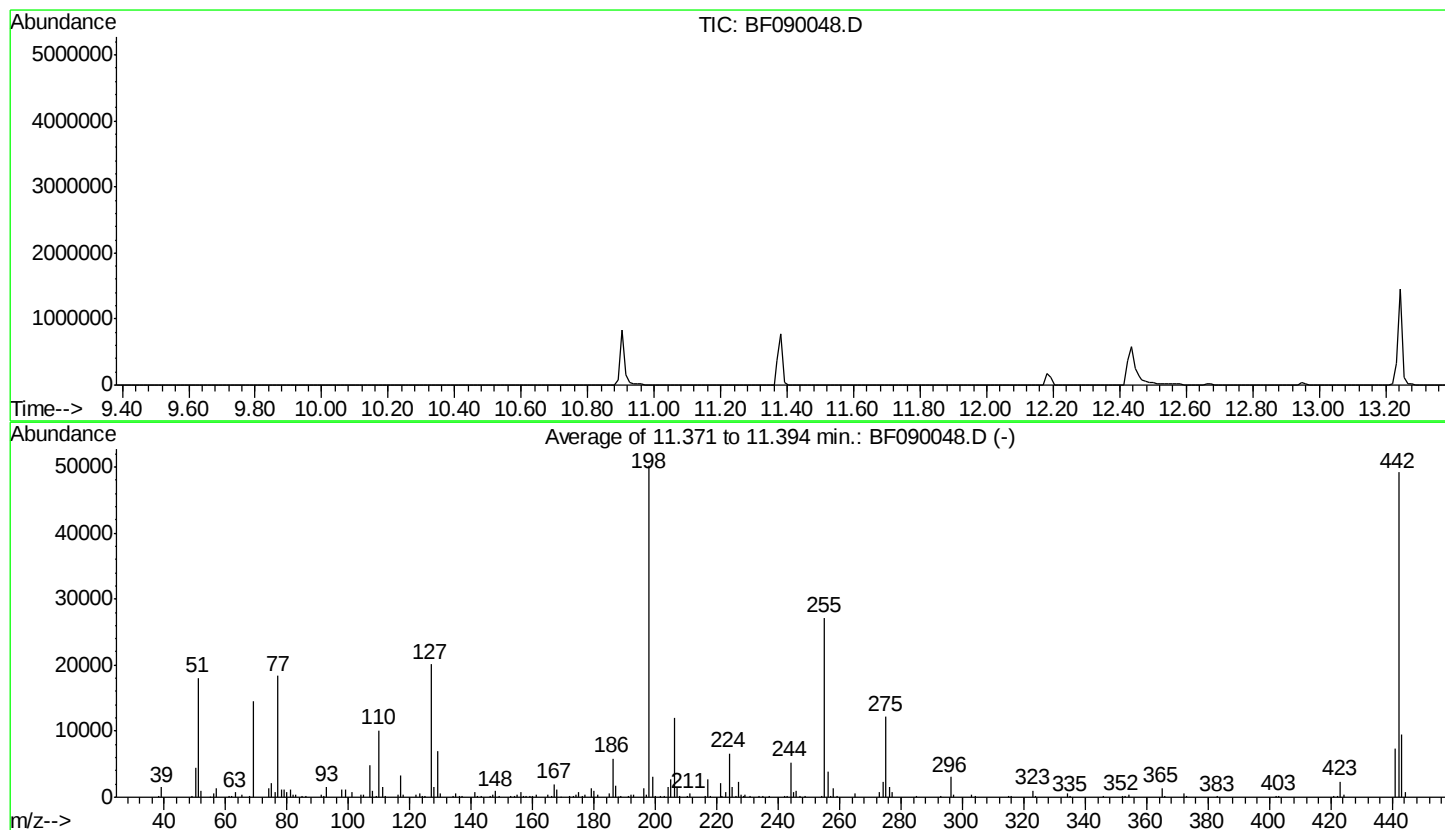

AutoFind: Scans 856, 857, 858; Background Corrected with Scan 852

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.0	18053	PASS
68	69	0.00	2	1.1	159	PASS
69	198	0.00	100	29.0	14558	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	40.1	20138	PASS
197	198	0.00	2	0.6	313	PASS
198	198	100	100	100.0	50187	PASS
199	198	5	9	6.3	3180	PASS
275	198	10	60	24.2	12134	PASS
365	198	1	100	2.8	1405	PASS
441	442	0.01	24	15.1	7438	PASS
442	198	50	100	98.0	49205	PASS
443	442	15	24	19.3	9495	PASS