
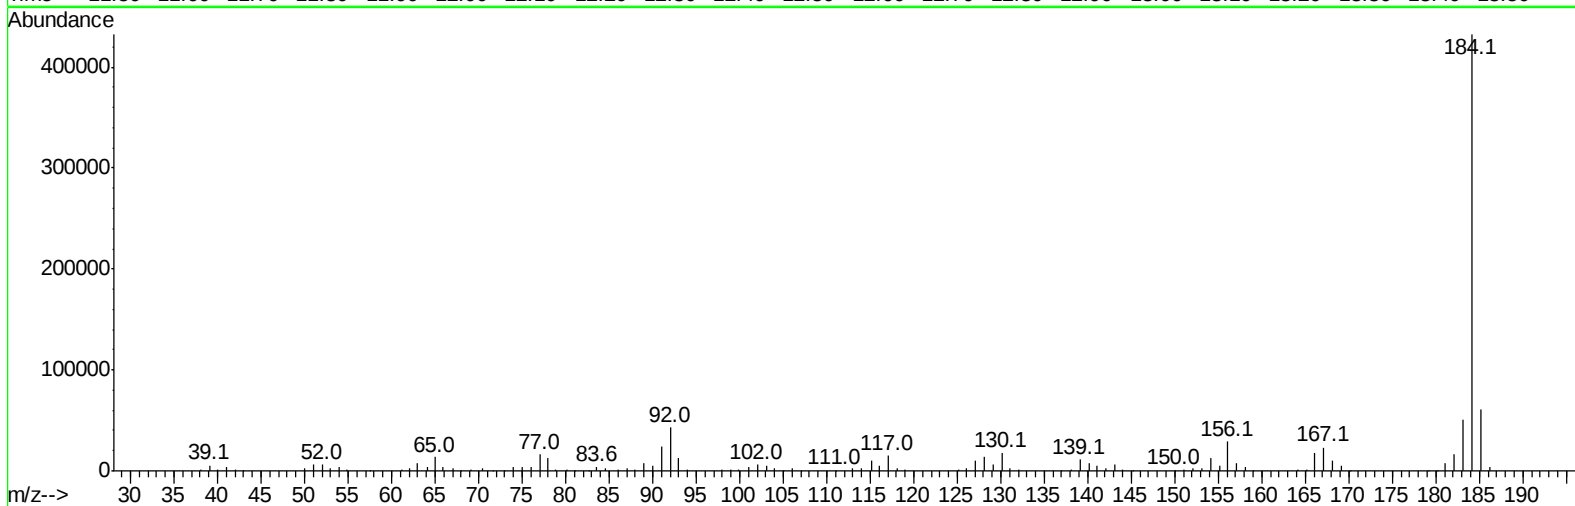


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090917\
 Data File : BF098376.D
 Acq On : 9 Sep 2017 10:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 07:31:40 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 05 17:28:20 2017
 Response via : Initial Calibration

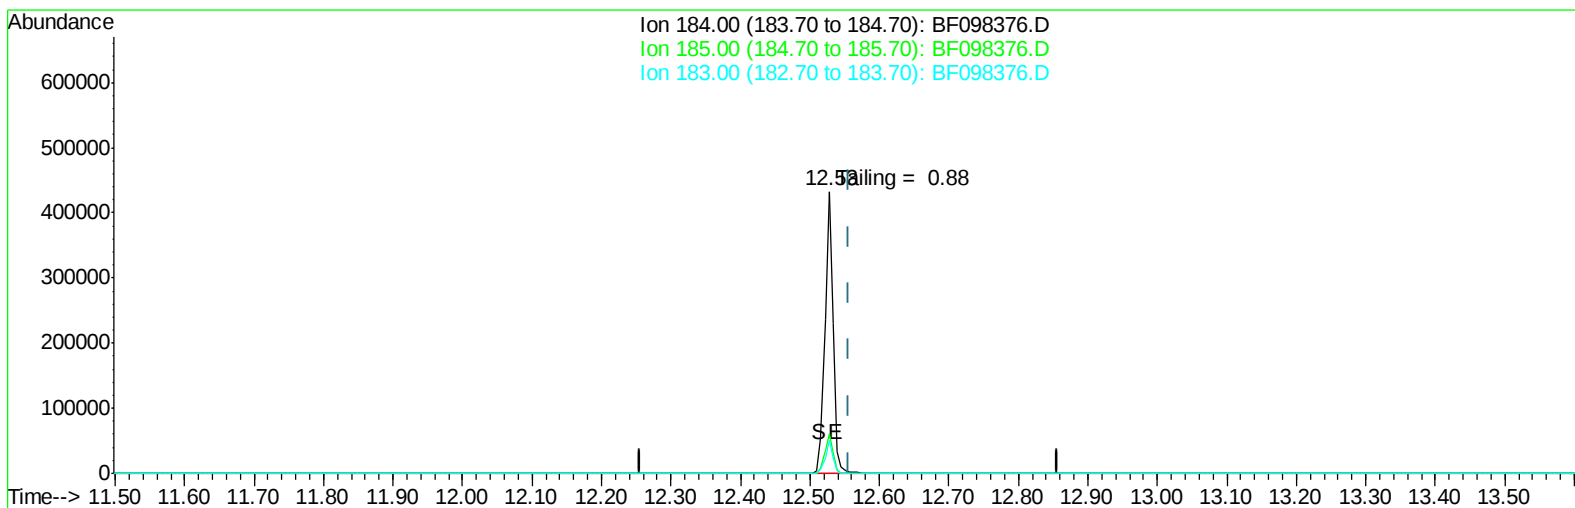

TIC: BF098376.D

(76) Benzidine



12.527min (-0.029) 0.00ng

response 358406

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.03#
183.00	12.20	11.75
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF090917\
Data File : BF098376.D
Acq On : 9 Sep 2017 10:14
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 11 07:31:40 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF081517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 05 17:28:20 2017
Response via : Initial Calibration

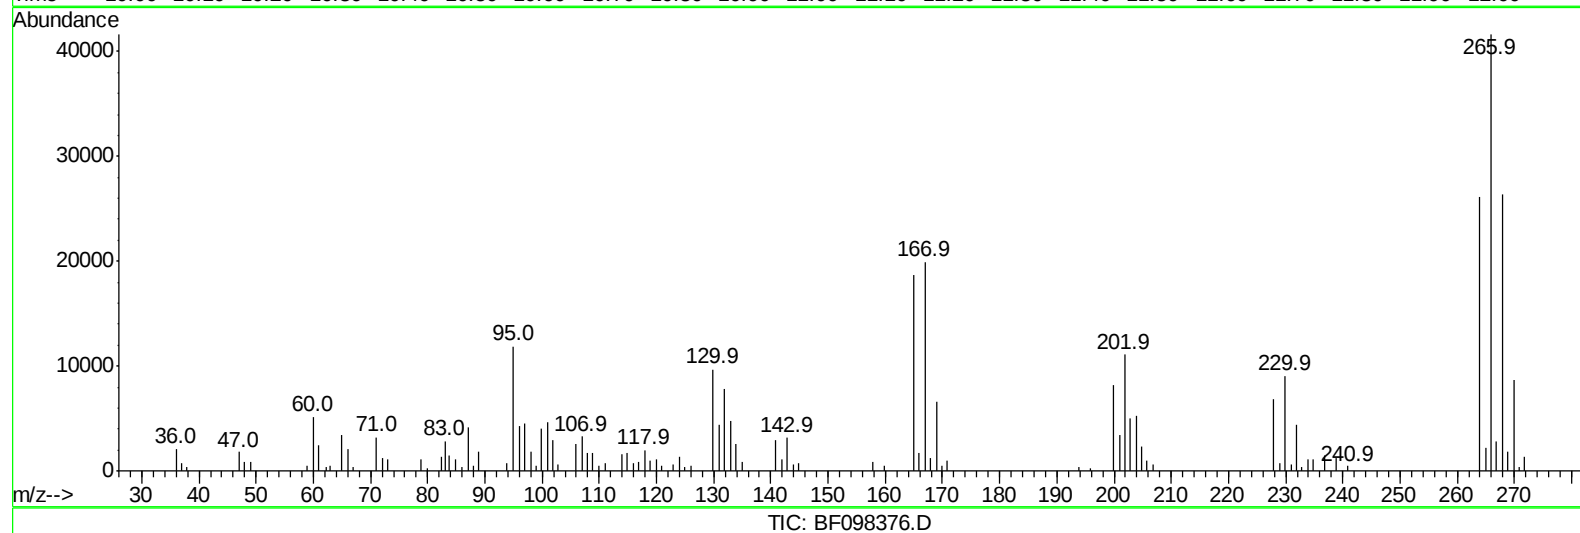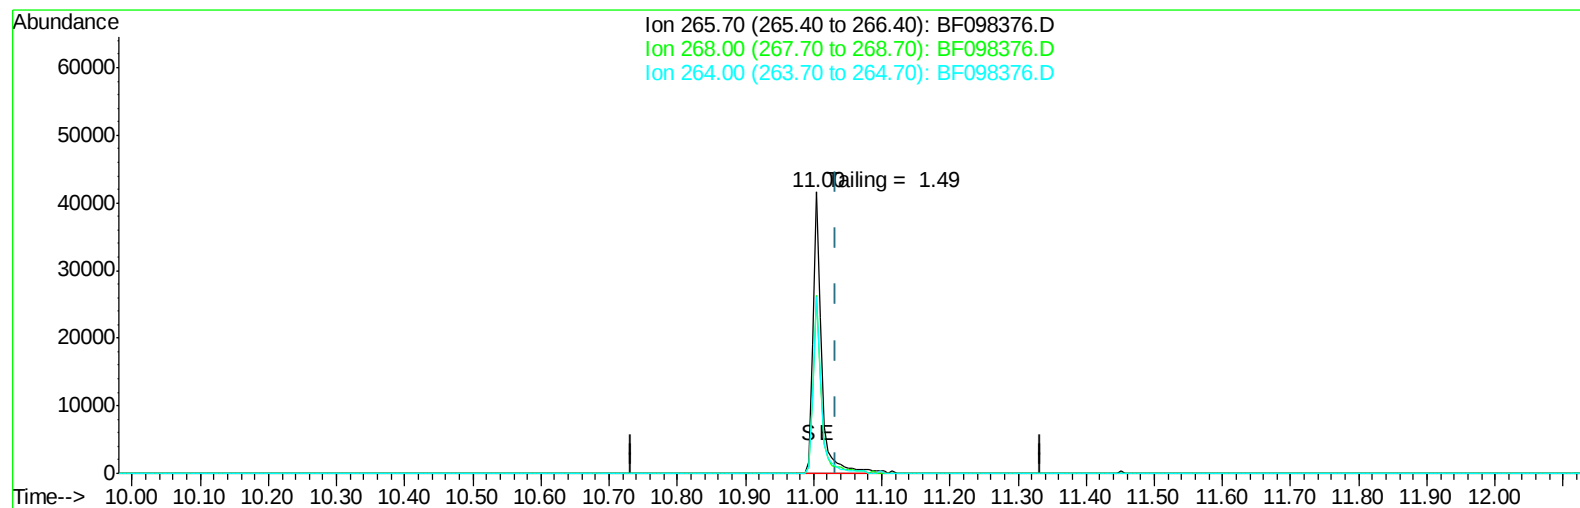

(69) Pentachlorophenol (C)

11.004min (-0.029) 24448.15ng

response 38021

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.42
264.00	64.60	62.86
0.00	0.00	0.00