


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF090917\
 Data File : BF098376.D
 Acq On : 9 Sep 2017 10:14
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF081517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 05 17:28:20 2017

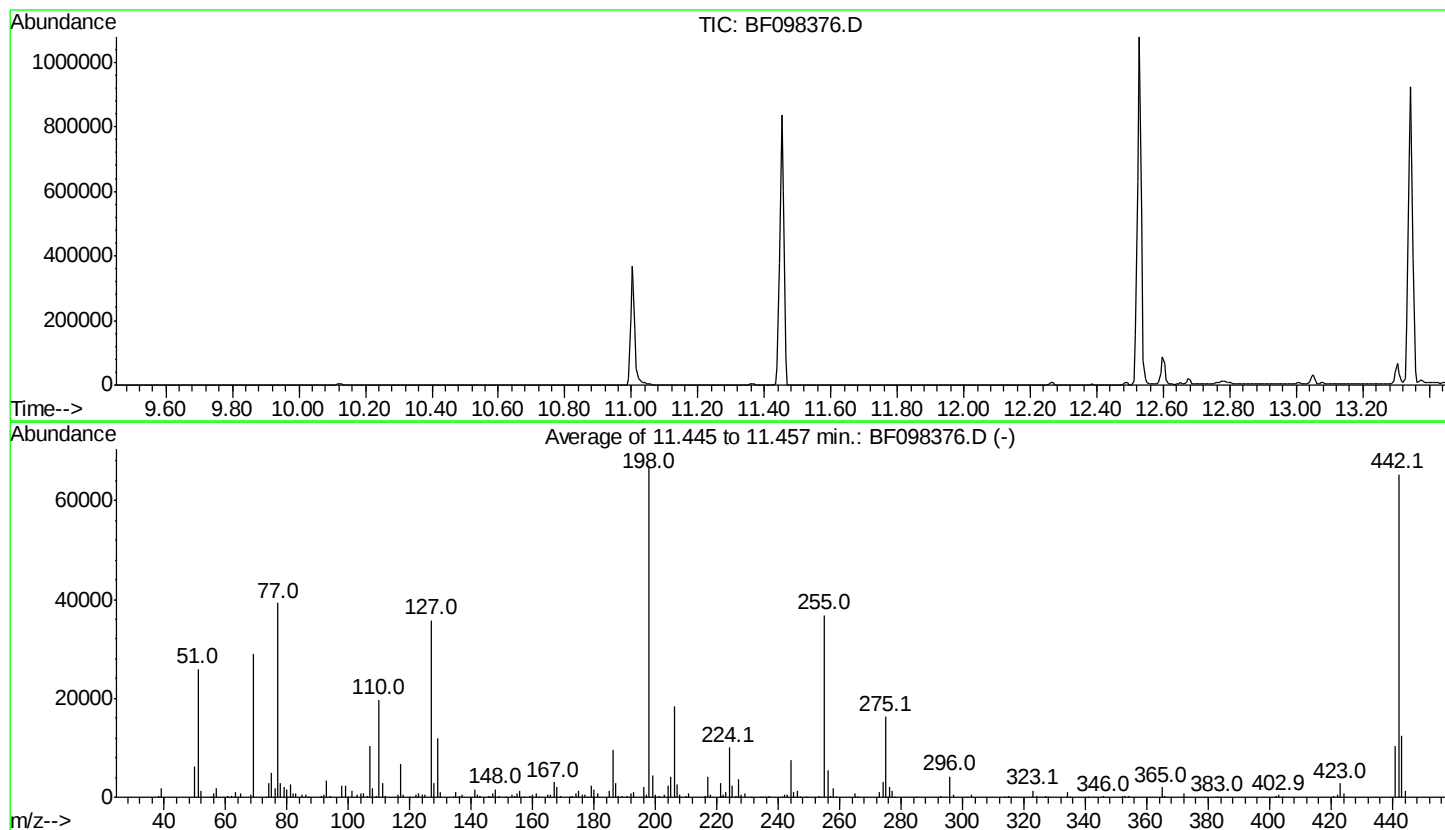

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	25914	PASS
68	69	0.00	2	1.9	538	PASS
69	198	0.00	100	43.2	29005	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.3	35744	PASS
197	198	0.00	2	0.8	562	PASS
198	198	100	100	100.0	67077	PASS
199	198	5	9	6.6	4455	PASS
275	198	10	60	24.2	16213	PASS
365	198	1	100	3.0	2022	PASS
441	442	0.01	24	15.7	10261	PASS
442	198	50	100	97.4	65362	PASS
443	442	15	24	19.0	12412	PASS