
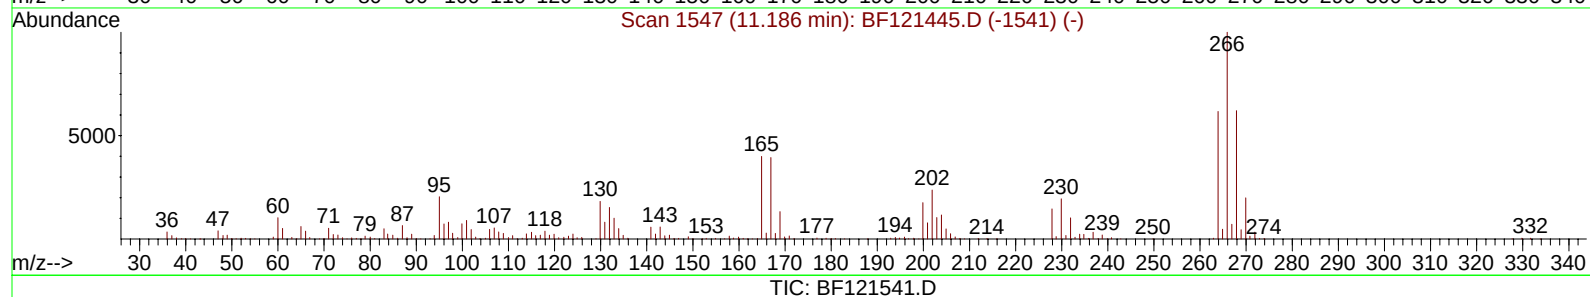
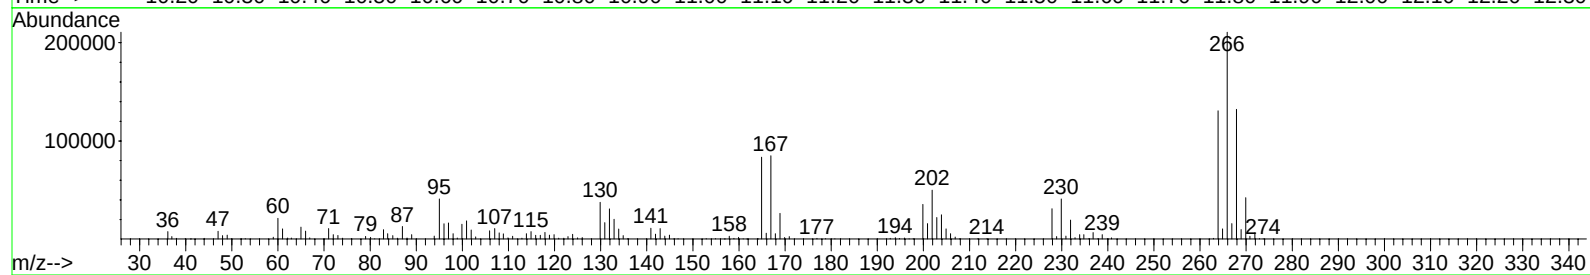


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090920\
Data File : BF121541.D
Acq On : 9 Sep 2020 11:04
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 16:37:59 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 02 17:52:18 2020
Response via : Initial Calibration

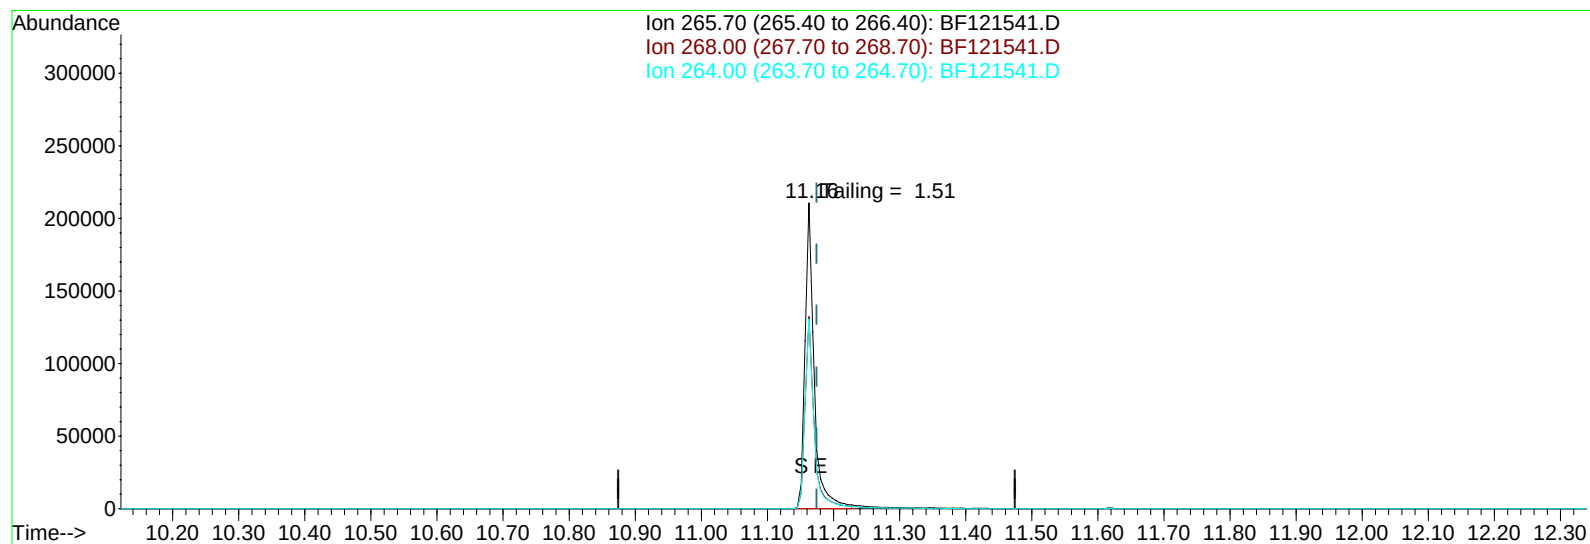

(70) Pentachlorophenol (C)




11.163min (-0.012) 43582.07ng

response 209773

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.78
264.00	62.60	62.06
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF090920\
 Data File : BF121541.D
 Acq On : 9 Sep 2020 11:04
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 09 16:37:59 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF082720.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 02 17:52:18 2020
 Response via : Initial Calibration

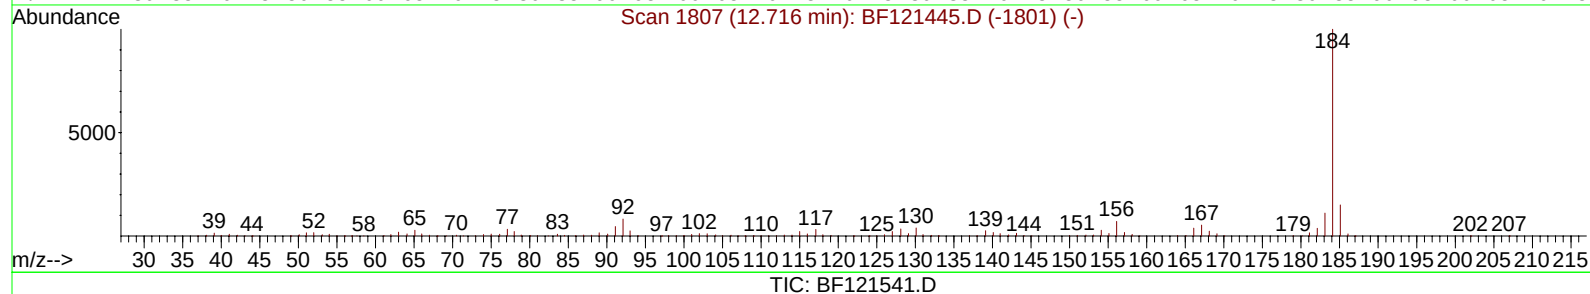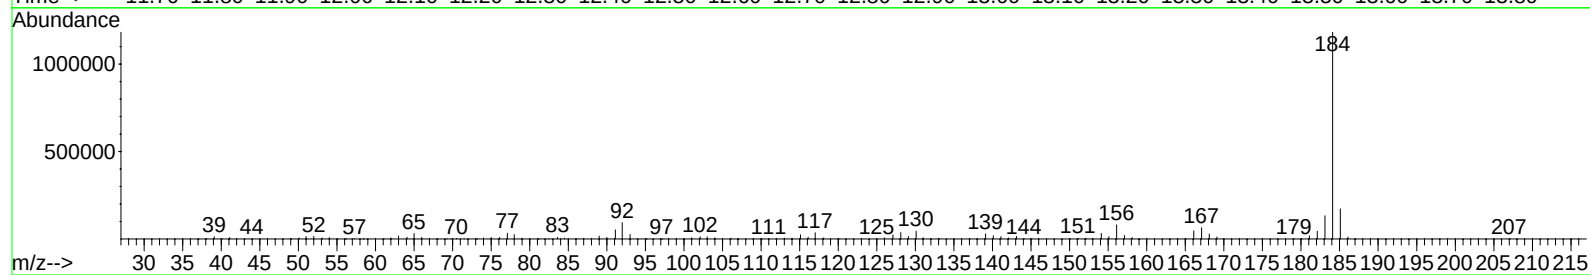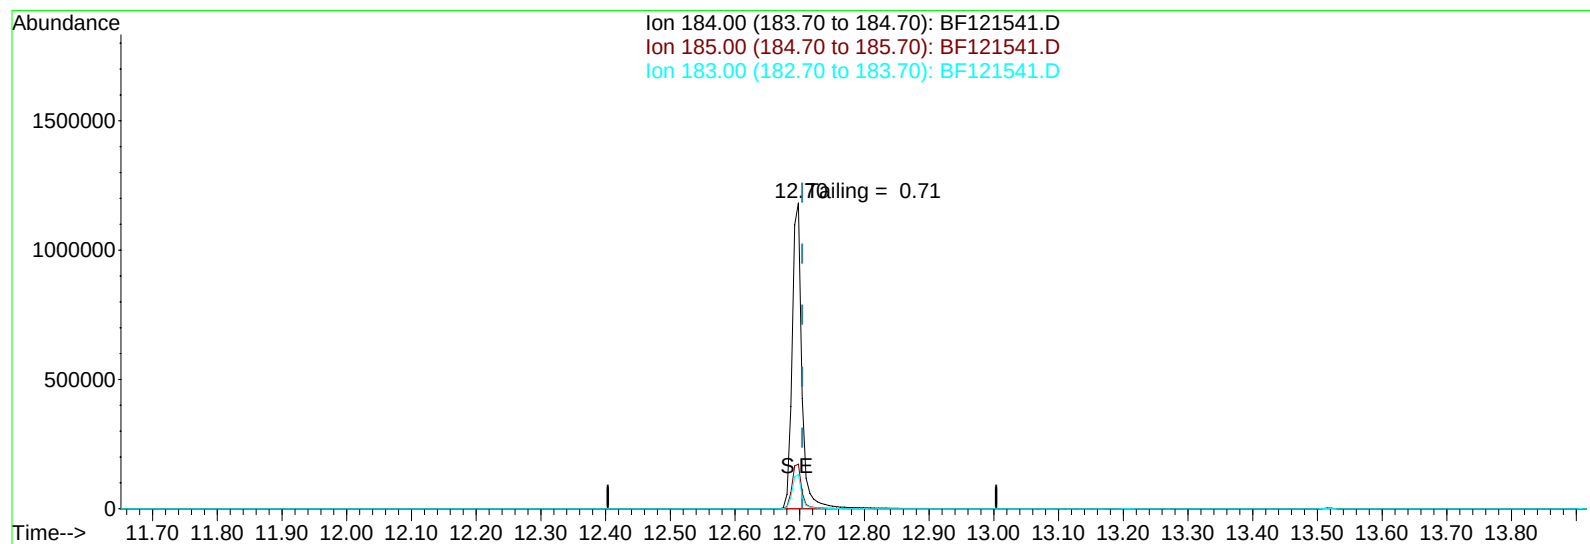

(77) Benzidine

12.698min (-0.006) 0.00ng

response 1249108

Ion	Exp%	Act%
184.00	100	100
185.00	14.40	14.62
183.00	11.30	11.25
0.00	0.00	0.00