
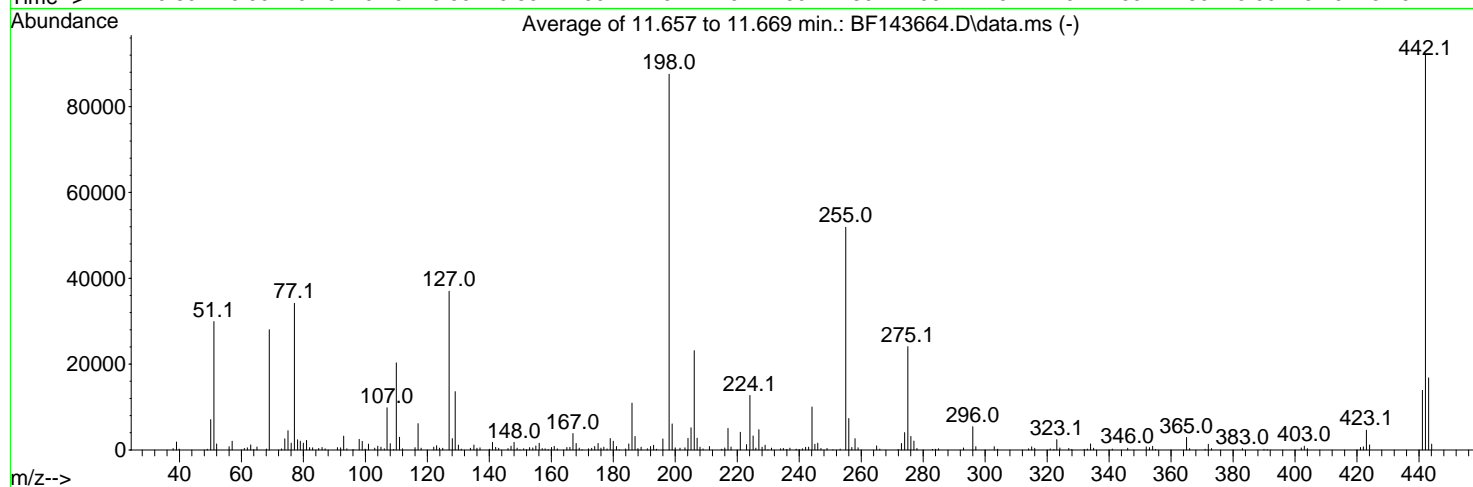


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF090925\
 Data File : BF143664.D
 Acq On : 08 Sep 2025 14:55
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090925.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 09 05:18:16 2025

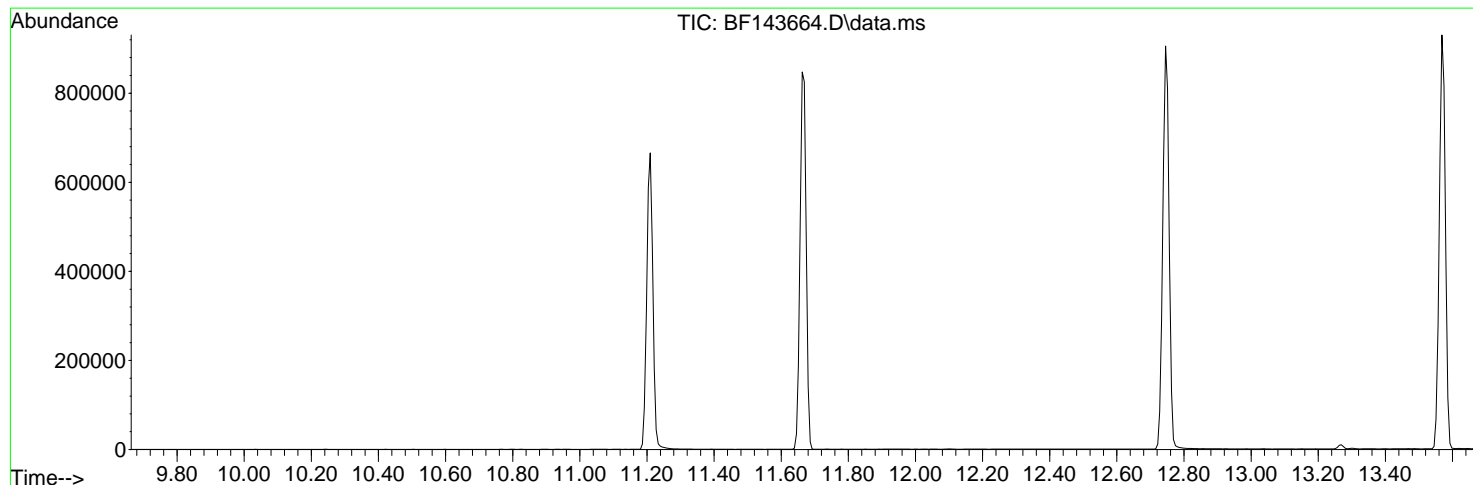

AutoFind: Scans 1609, 1610, 1611; Background Corrected with Scan 1603

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.7	202	PASS
69	69	100	100	100.0	28037	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	87563	PASS
199	198	5	9	6.9	6062	PASS
365	198	1	100	3.3	2914	PASS
441	443	0.01	150	82.5	13878	PASS
442	442	100	100	100.0	92013	PASS
443	442	15	24	18.3	16813	PASS