
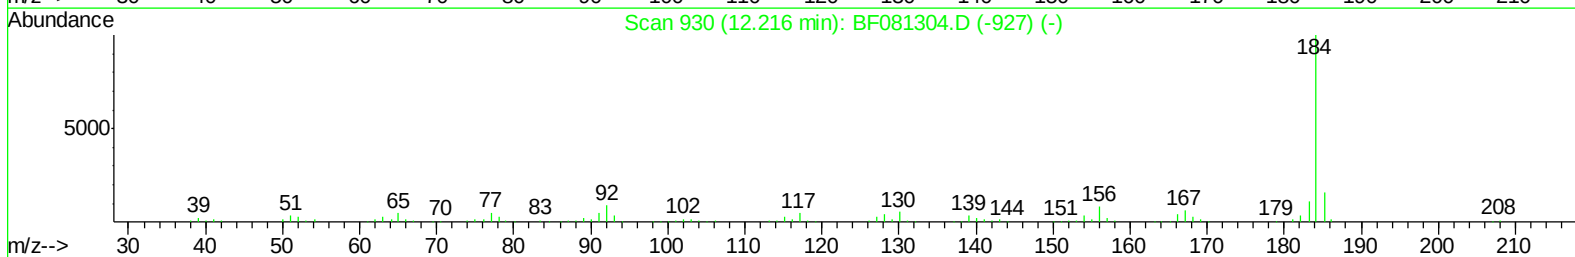
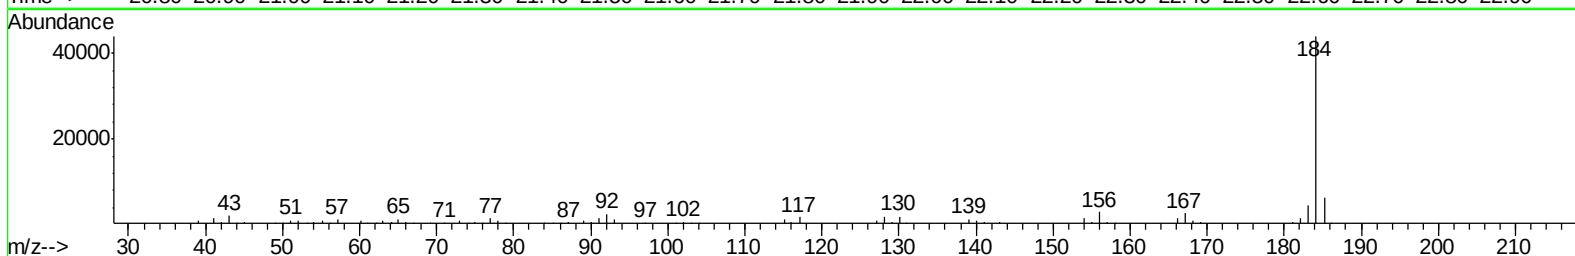


Data Path : Z:\HPCHEM1\BNA_F\Data\BF091015\
Data File : BF081568.D
Acq On : 10 Sep 2015 14:18
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 17:35:31 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 10 16:31:29 2015
Response via : Initial Calibration

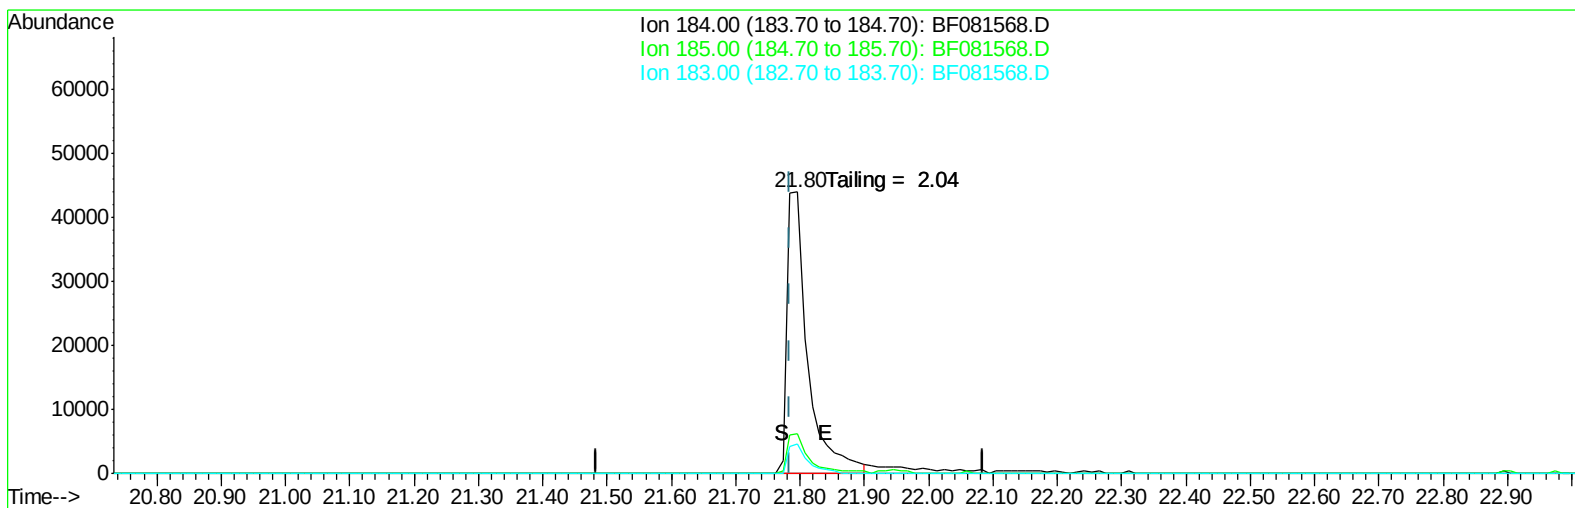

TIC: BF081568.D

(76) Benzidine




21.796min (+0.011) 0.00ng m

response 92571

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	14.10
183.00	9.50	10.52
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF091015\
Data File : BF081568.D
Acq On : 10 Sep 2015 14:18
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 17:35:31 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 10 16:31:29 2015
Response via : Initial Calibration

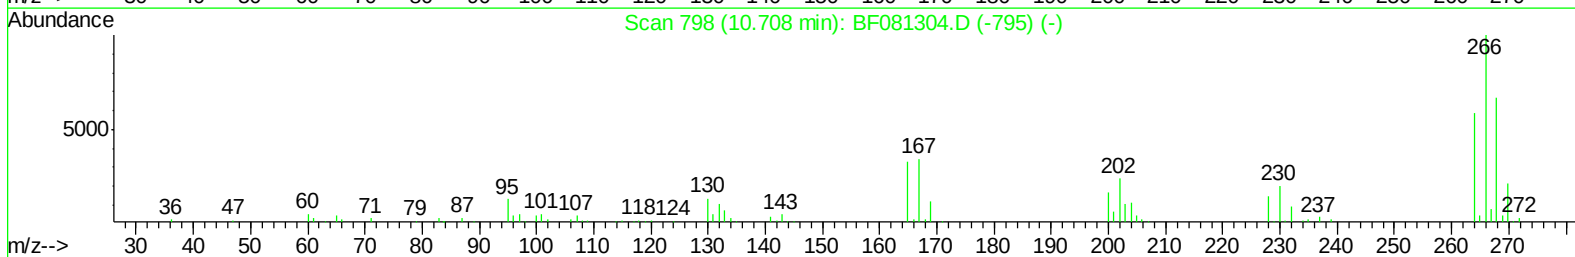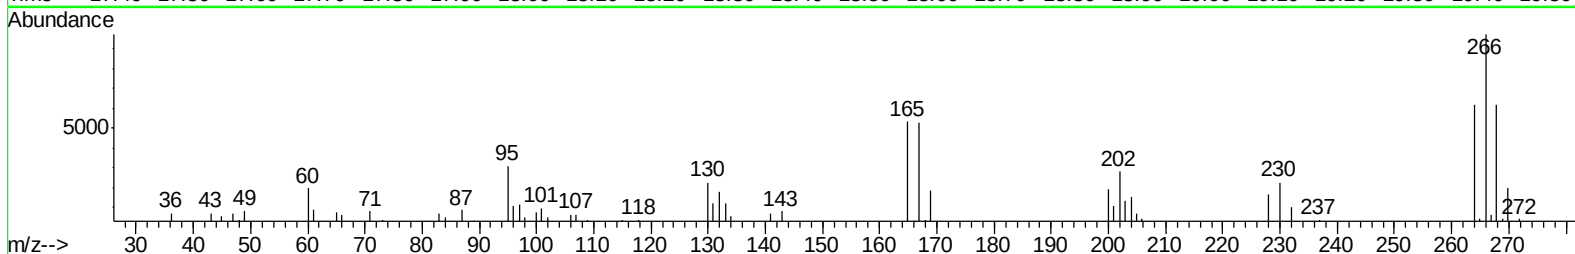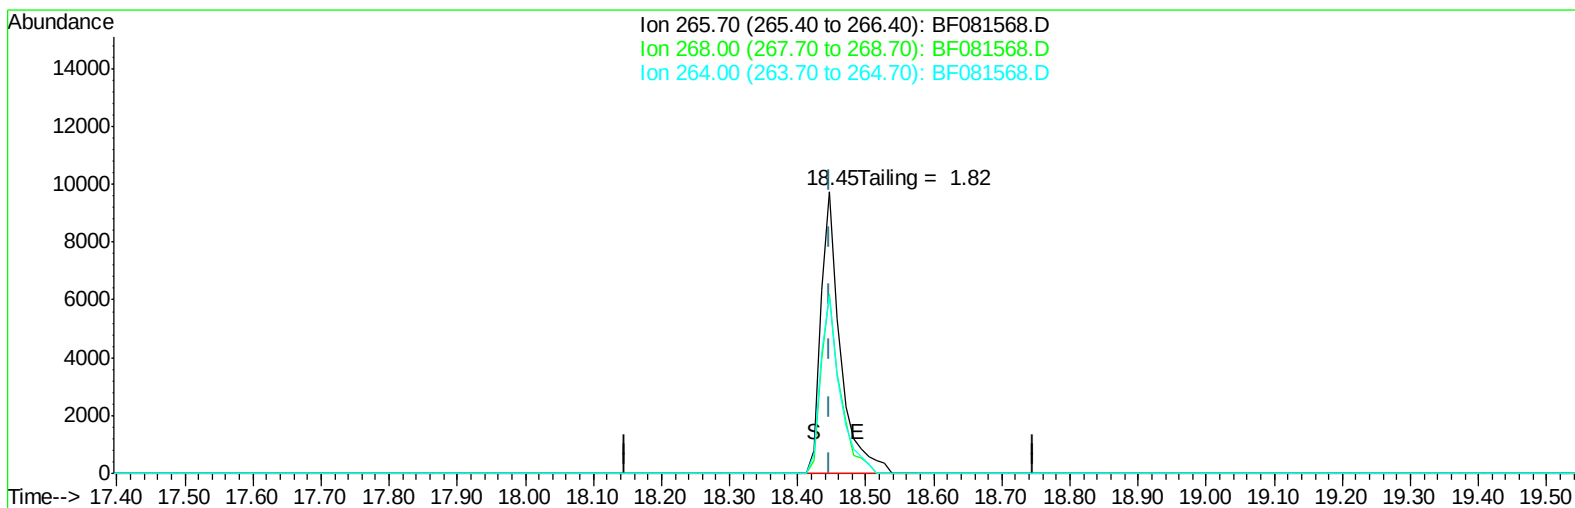

TIC: BF081568.D

(69) Pentachlorophenol (C)

18.447min (0.000) 0.00ng

response 19108

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.74
264.00	62.70	63.28
0.00	0.00	0.00