

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091018\
 Data File : BF108898.D
 Acq On : 10 Sep 2018 17:37
 Operator : JU/SJ
 Sample : J4777-09 5X
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PL-05-090718-E

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF090518.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.919	436	439	445	rBV	25836	27935	1.76%	0.194%
2	5.342	507	511	519	rBV	697237	637035	40.14%	4.428%
3	6.366	681	685	691	rBV	800048	676411	42.62%	4.701%
4	6.501	705	708	712	rBV	792389	683837	43.08%	4.753%
5	6.742	745	749	752	rBV	1434521	1255844	79.12%	8.729%
6	6.895	771	775	778	rBV	733832	551430	34.74%	3.833%
7	7.295	839	843	846	rBV	450289	389561	24.54%	2.708%
8	8.019	963	966	970	rBV	1715638	1551406	97.74%	10.783%
9	9.095	1145	1149	1152	rBV	992864	748541	47.16%	5.203%
10	9.489	1212	1216	1219	rBV	173940	157269	9.91%	1.093%
11	9.630	1237	1240	1246	rBV	55442	53565	3.37%	0.372%
12	9.772	1260	1264	1268	rBV	1781010	1480413	93.27%	10.290%
13	10.554	1393	1397	1402	rBV	302612	289802	18.26%	2.014%
14	10.701	1416	1422	1426	rVB2	51387	71483	4.50%	0.497%
15	11.166	1498	1501	1505	rVB	60809	57195	3.60%	0.398%
16	11.248	1511	1515	1518	rBV	1502316	1237083	77.94%	8.598%
17	11.271	1518	1519	1522	rVV	141696	75561	4.76%	0.525%
18	11.324	1525	1528	1531	rVB	64942	57316	3.61%	0.398%
19	11.748	1598	1600	1603	rBV2	31311	27686	1.74%	0.192%
20	11.777	1603	1605	1608	rVV2	49777	45074	2.84%	0.313%
21	11.860	1616	1619	1621	rBV	82373	83974	5.29%	0.584%
22	12.301	1691	1694	1696	rBV	51585	55371	3.49%	0.385%
23	12.336	1698	1700	1702	rBV2	50600	40827	2.57%	0.284%
24	12.454	1717	1720	1724	rBV	492222	433698	27.32%	3.014%
25	12.683	1754	1759	1762	rBV	689915	641116	40.39%	4.456%
26	12.830	1781	1784	1791	rVB	694855	618294	38.95%	4.297%
27	13.113	1830	1832	1834	rBV	86183	83623	5.27%	0.581%
28	13.236	1851	1853	1856	rBV	91262	82702	5.21%	0.575%
29	13.877	1958	1962	1965	rBV2	1523618	1587215	100.00%	11.032%
30	15.289	2199	2202	2206	rVB	599625	686279	43.24%	4.770%


Sum of corrected areas: 14387546

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091018\
Data File : BF108898.D
Acq On : 10 Sep 2018 17:37
Operator : JU/SJ
Sample : J4777-09 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PL-05-090718-E

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

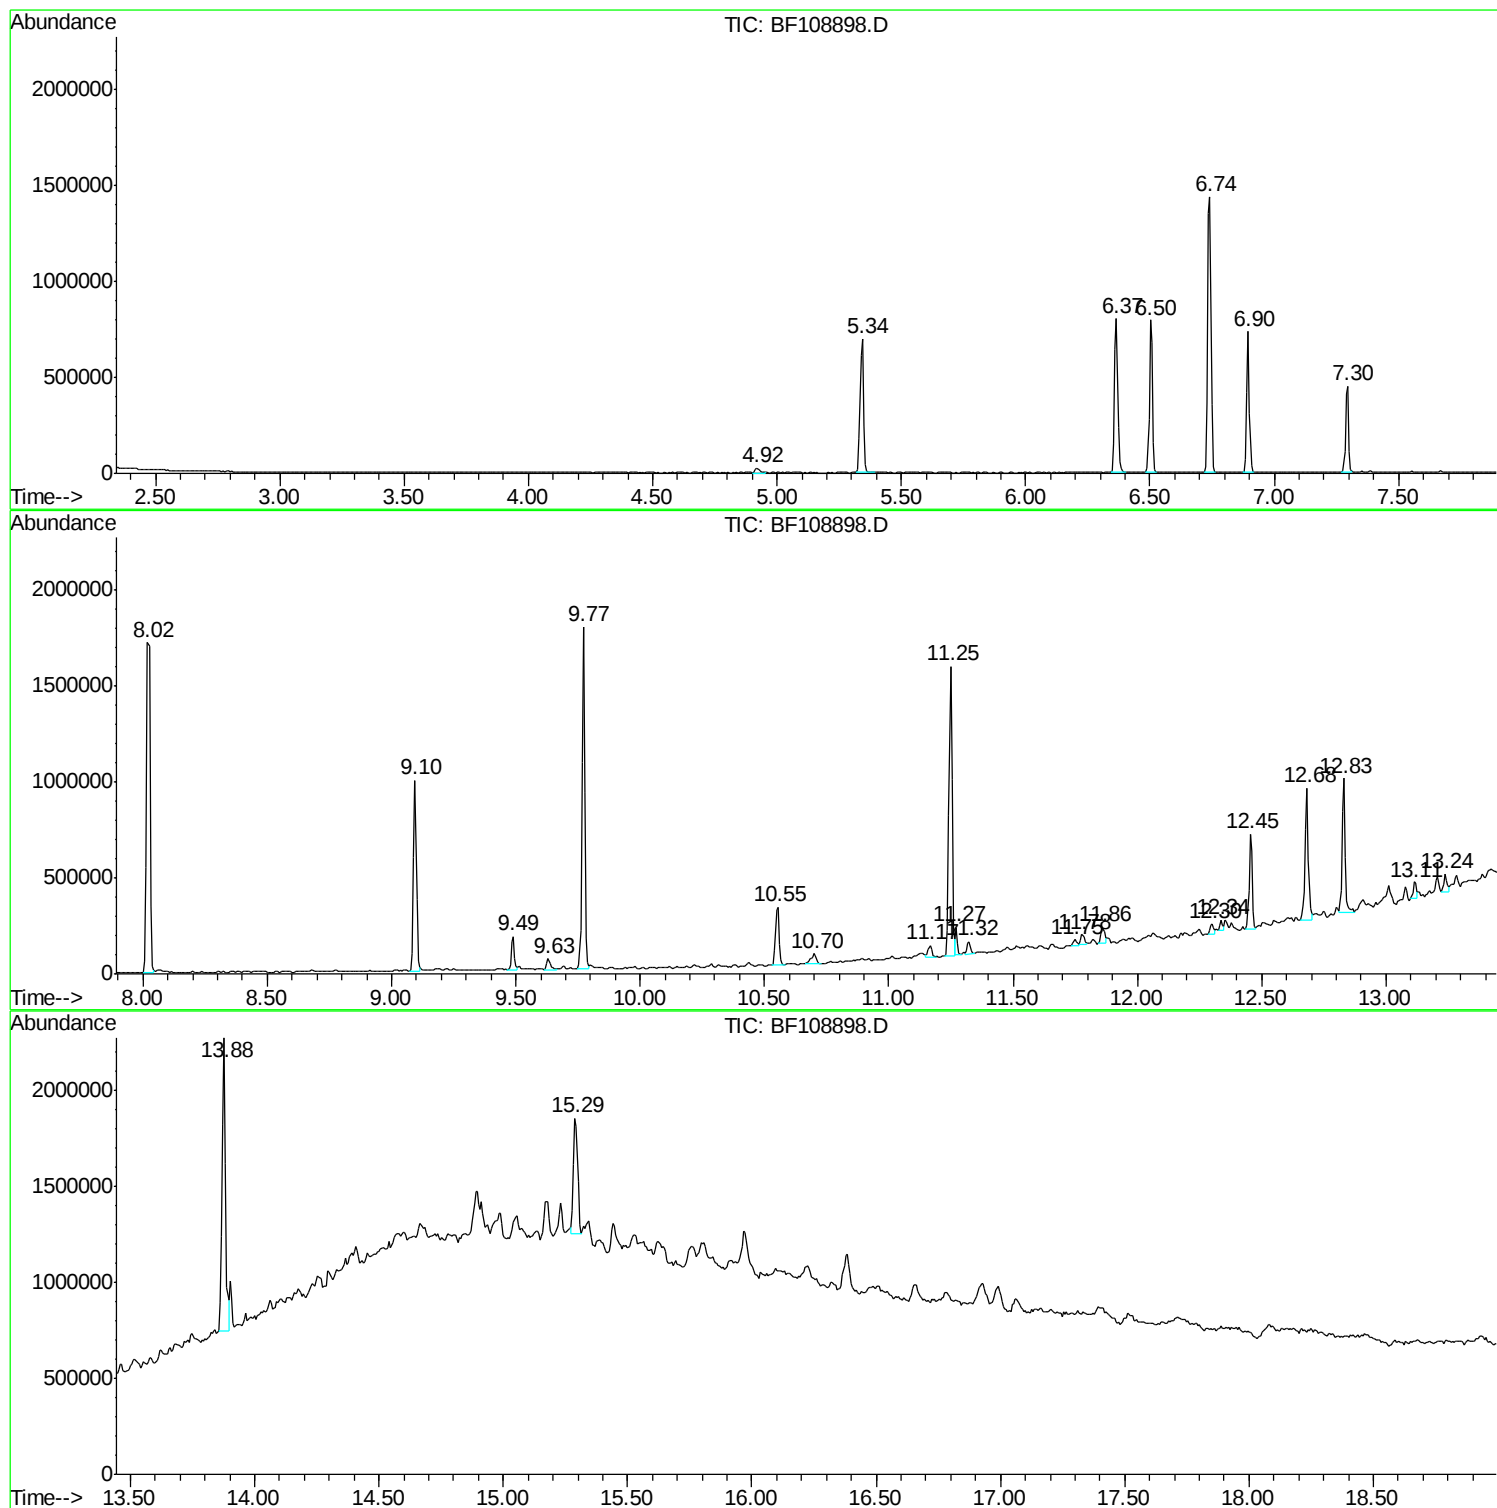

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091018\
Data File : BF108898.D
Acq On : 10 Sep 2018 17:37
Operator : JU/SJ
Sample : J4777-09 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PL-05-090718-E










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF090518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.50 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.50	10.89 ng	683837	1,4-Dichlorobenzene-d4	6.74

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		5-Aminoindole	132	C8H8N2	005192-03-0	10
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

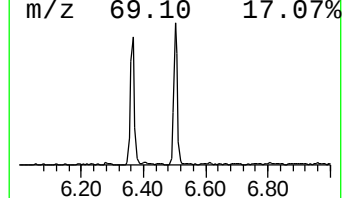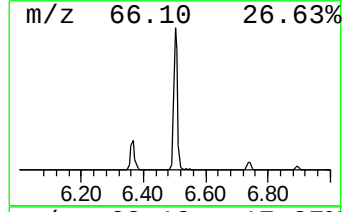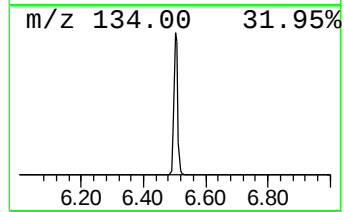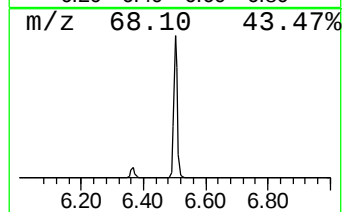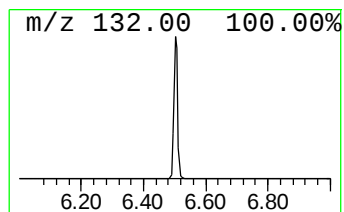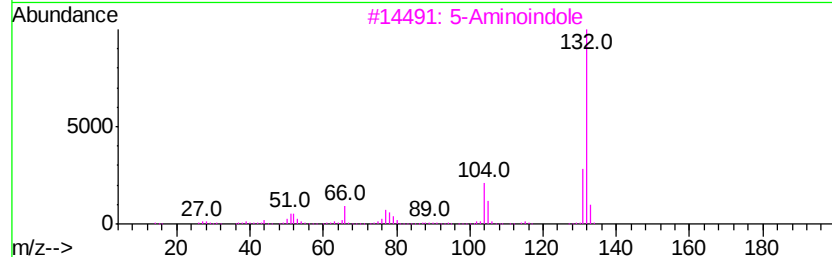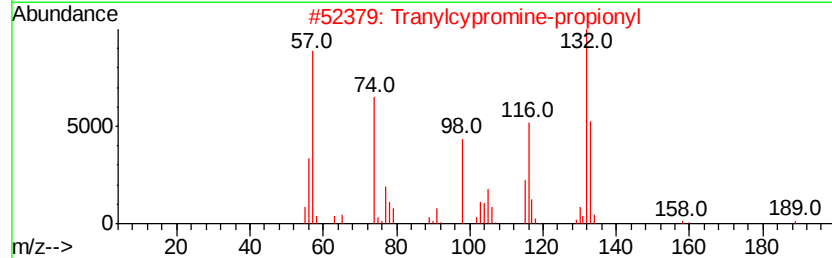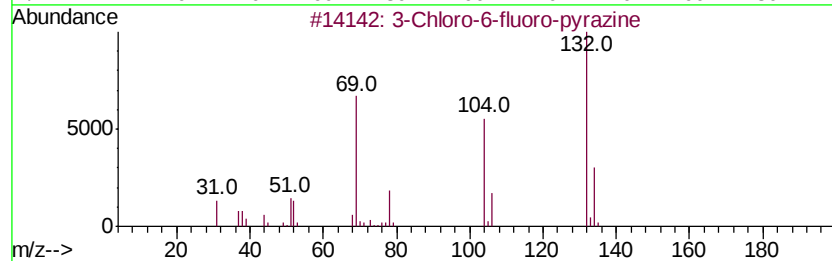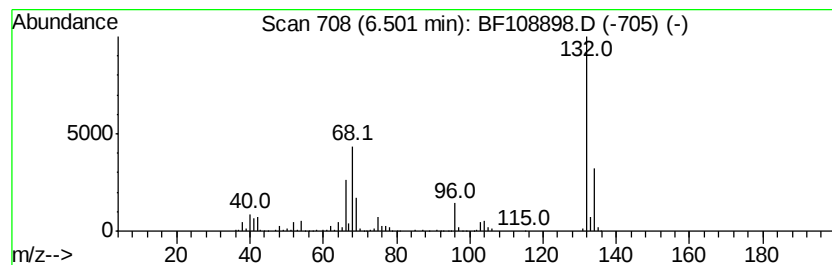

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091018\
Data File : BF108898.D
Acq On : 10 Sep 2018 17:37
Operator : JU/SJ
Sample : J4777-09 5X
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PL-05-090718-E

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF090518.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.50	6.50	10.9	ng	683837	1	6.74	1255840	20.0