


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091018\
 Data File : BF108886.D
 Acq On : 10 Sep 2018 12:11
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF090518.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 05 18:03:31 2018

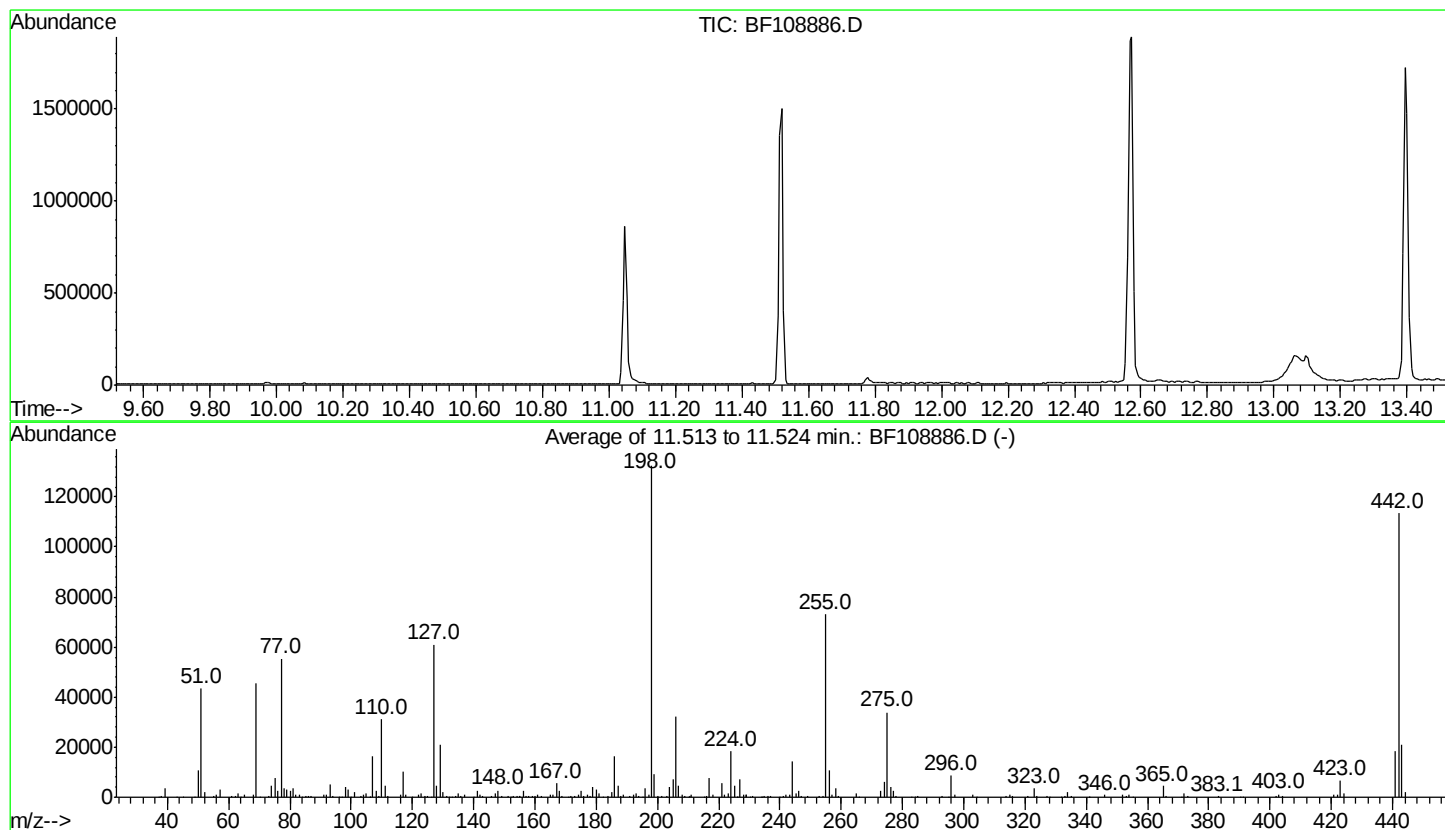

AutoFind: Scans 1560, 1561, 1562; Background Corrected with Scan 1555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	43314	PASS
68	69	0.00	2	2.0	891	PASS
69	198	0.00	100	34.2	45307	PASS
70	69	0.00	2	0.5	226	PASS
127	198	10	80	46.1	61084	PASS
197	198	0.00	2	0.7	864	PASS
198	198	100	100	100.0	132469	PASS
199	198	5	9	7.0	9248	PASS
275	198	10	60	25.5	33789	PASS
365	198	1	100	3.3	4378	PASS
441	198	0.01	100	13.7	18201	PASS
442	198	50	100	85.6	113354	PASS
443	442	15	24	18.4	20893	PASS