


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF091018\  
 Data File : BF108913.D  
 Acq On : 11 Sep 2018 00:45  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF090518.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Sep 05 18:03:31 2018

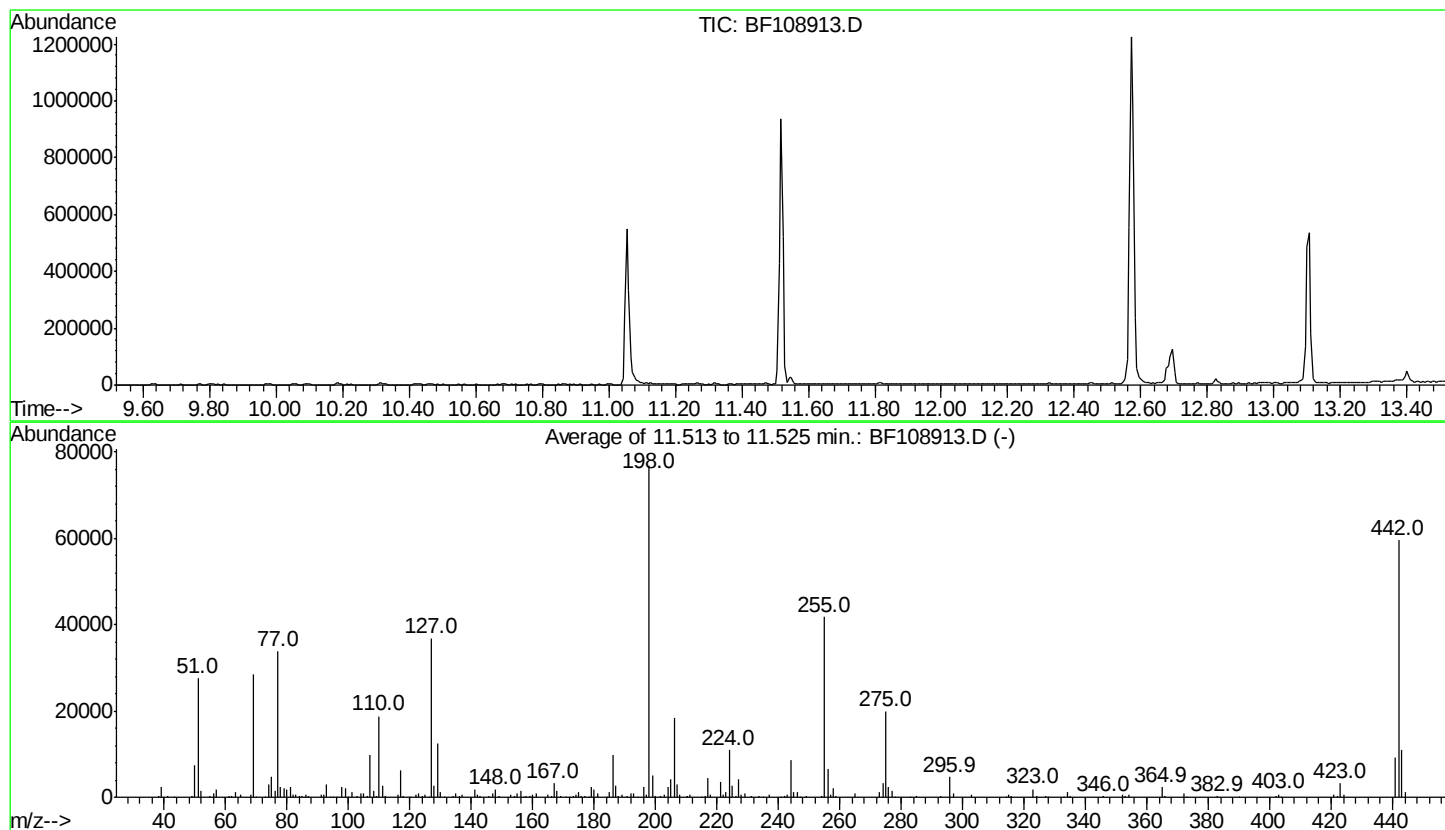

AutoFind: Scans 1560, 1561, 1562; Background Corrected with Scan 1556

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 35.9      | 27555   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 465     | PASS             |
| 69          | 198          | 0.00         | 100          | 37.1      | 28481   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 104     | PASS             |
| 127         | 198          | 10           | 80           | 47.7      | 36648   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.8       | 602     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 76805   | PASS             |
| 199         | 198          | 5            | 9            | 6.8       | 5191    | PASS             |
| 275         | 198          | 10           | 60           | 25.7      | 19731   | PASS             |
| 365         | 198          | 1            | 100          | 2.9       | 2265    | PASS             |
| 441         | 198          | 0.01         | 100          | 12.1      | 9280    | PASS             |
| 442         | 198          | 50           | 100          | 77.5      | 59498   | PASS             |
| 443         | 442          | 15           | 24           | 18.3      | 10908   | PASS             |