
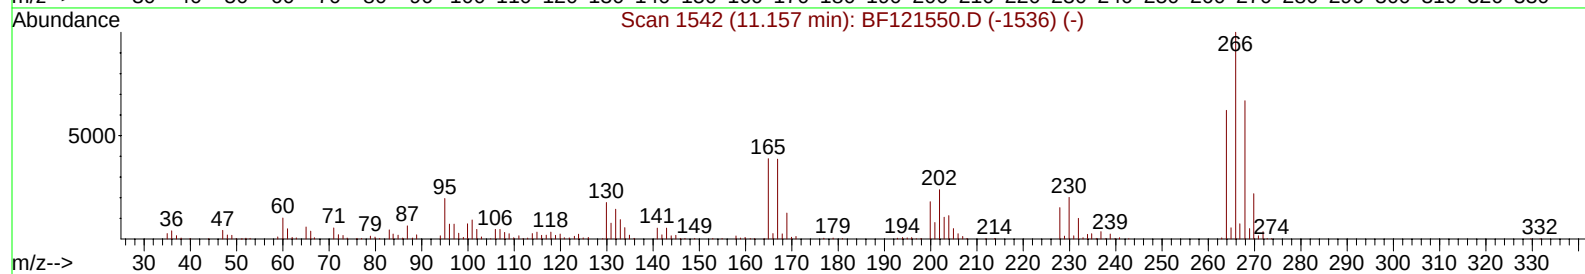
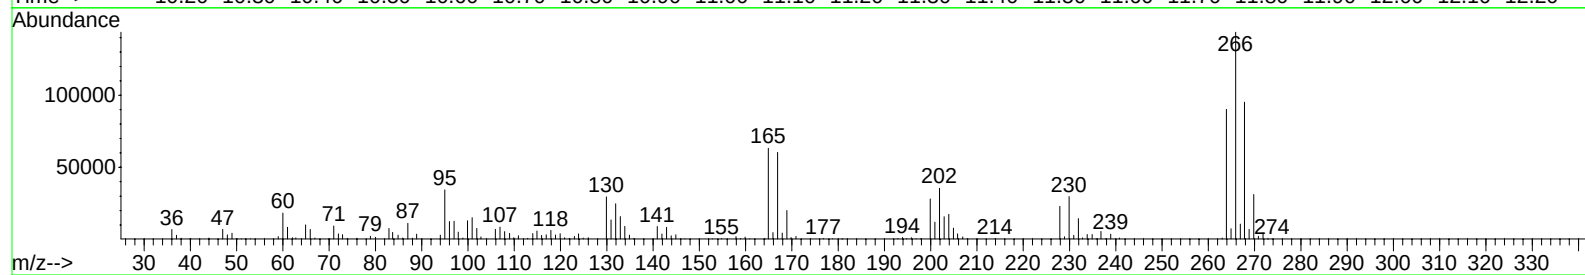


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091020\
 Data File : BF121546.D
 Acq On : 10 Sep 2020 12:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 18:01:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 10 16:47:54 2020
 Response via : Initial Calibration

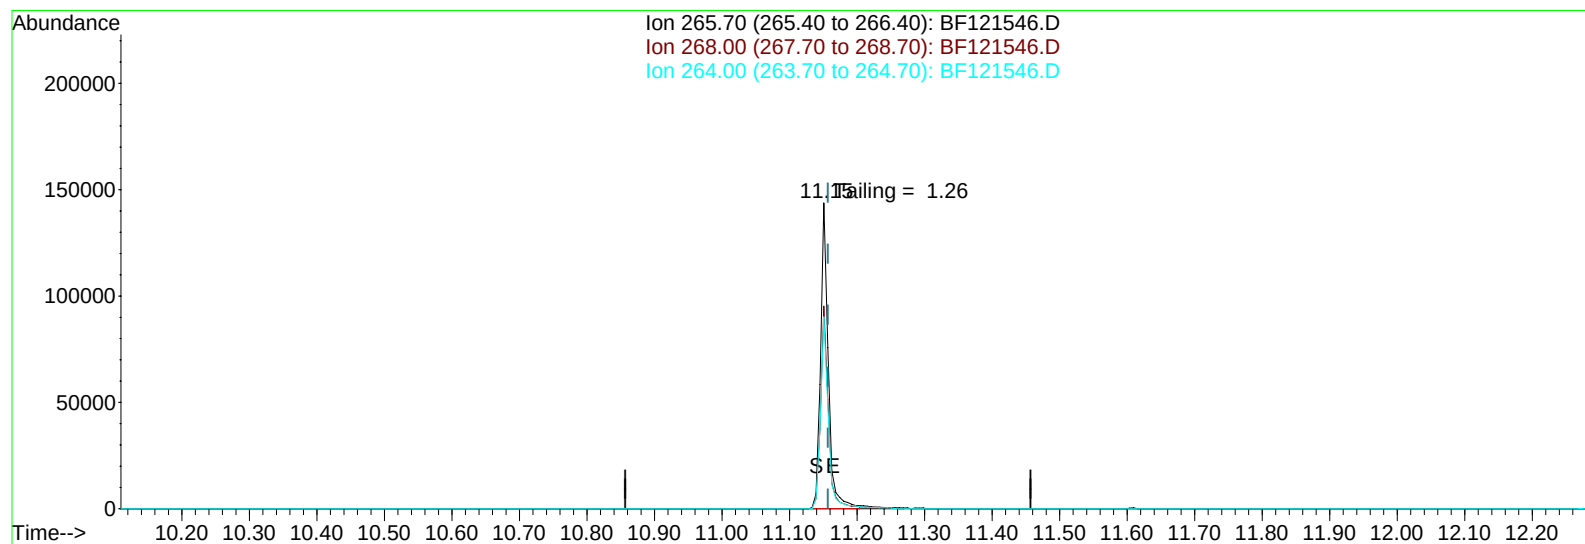

TIC: BF121546.D

(70) Pentachlorophenol (C)




11.151min (-0.006) 34998.38ng

response 118542

Ion	Exp%	Act%
265.70	100	100
268.00	66.90	66.26
264.00	62.30	62.76
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091020\
 Data File : BF121546.D
 Acq On : 10 Sep 2020 12:05
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 18:01:41 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF091020.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 10 16:47:54 2020
 Response via : Initial Calibration

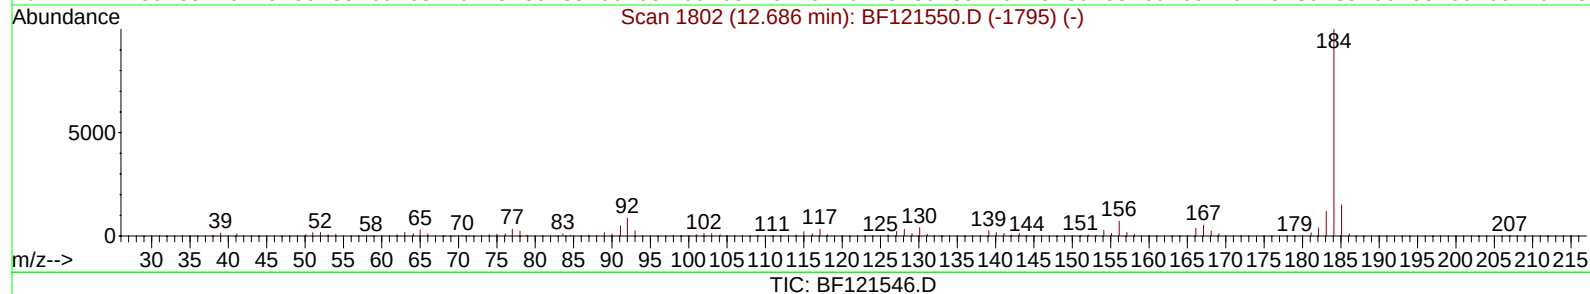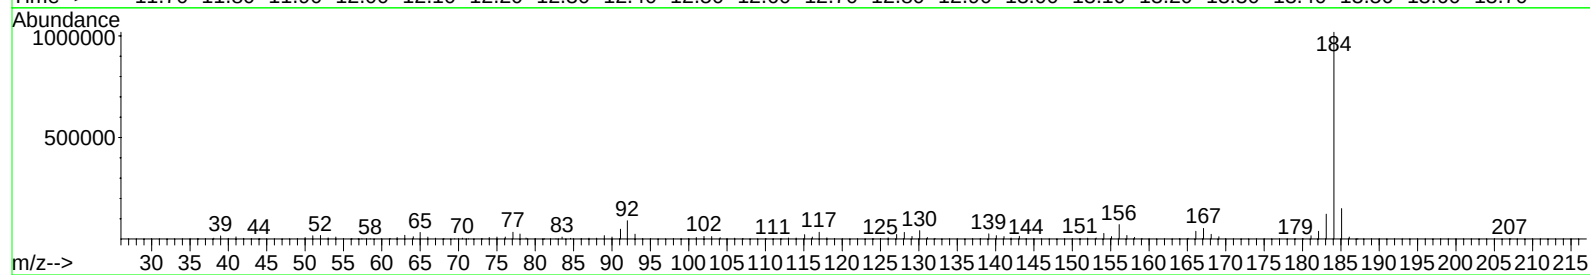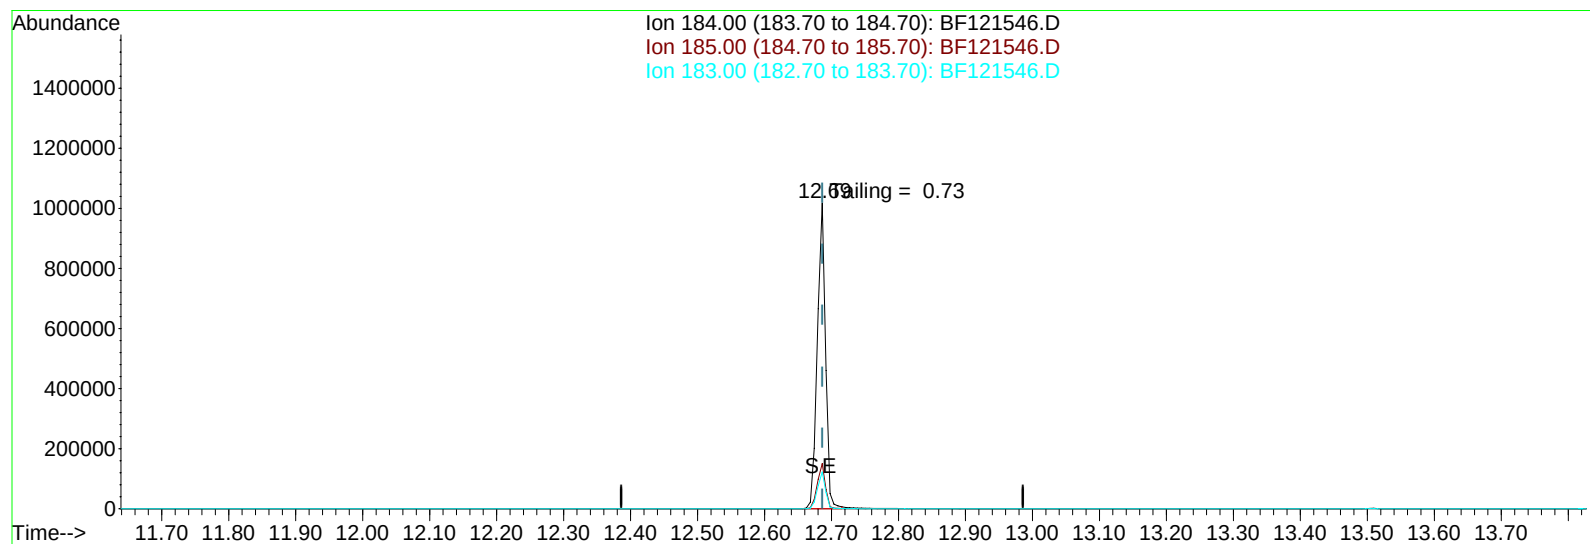

(77) Benzidine

12.686min (-0.000) 0.00ng

response 875302

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.76
183.00	11.90	12.02
0.00	0.00	0.00