
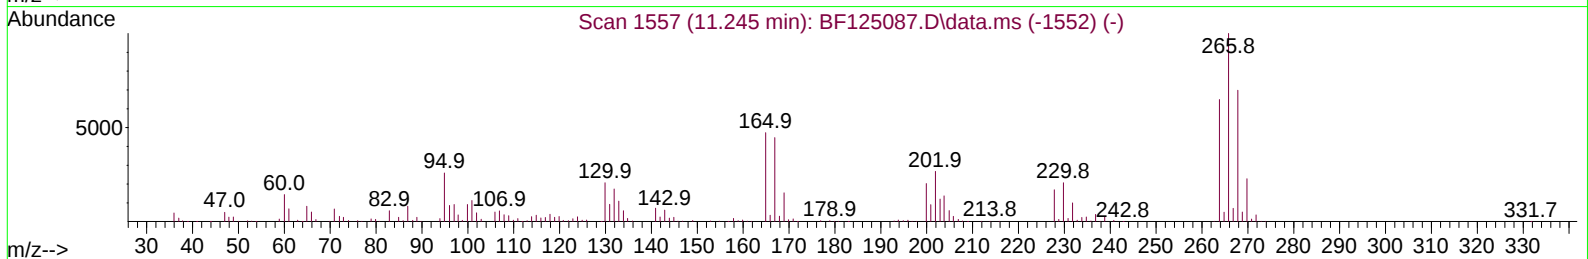
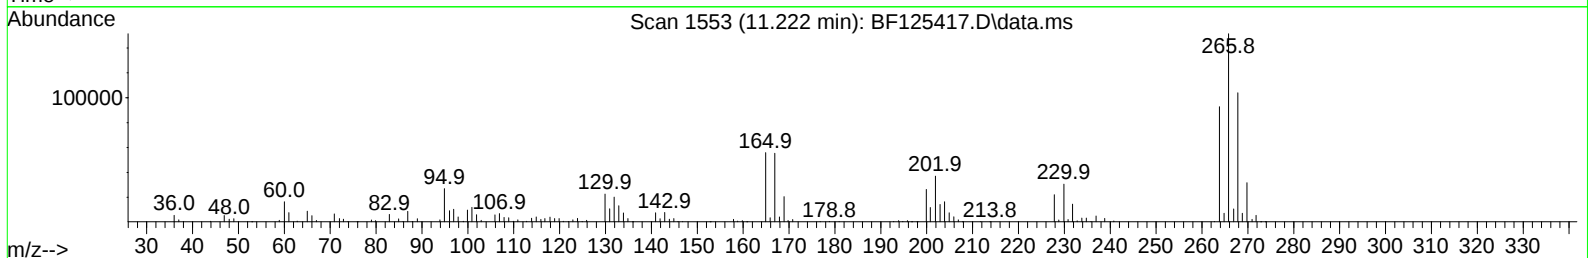


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091021\
 Data File : BF125417.D
 Acq On : 10 Sep 2021 10:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 13:10:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 08 14:14:01 2021
 Response via : Initial Calibration

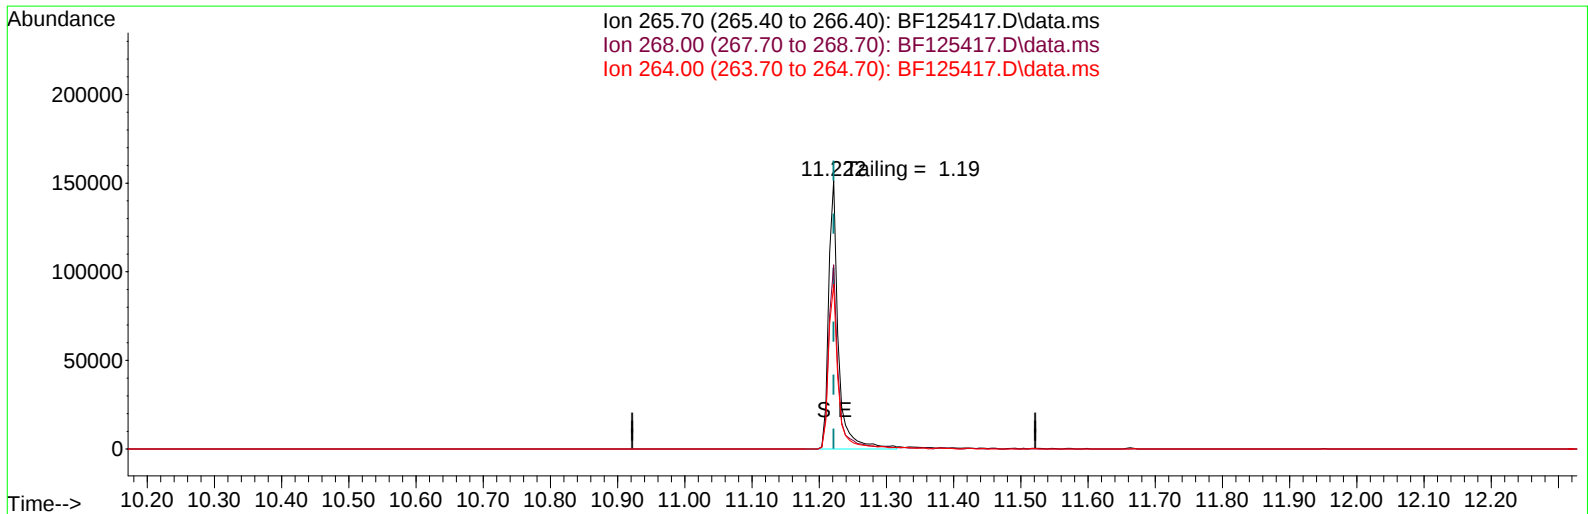

TIC: BF125417.D\data.ms

(70) Pentachlorophenol (C)




11.222min (+ 0.000) 26317.11 ng

response 153190

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.63
264.00	69.90	61.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091021\
Data File : BF125417.D
Acq On : 10 Sep 2021 10:11
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 10 13:10:55 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 08 14:14:01 2021
Response via : Initial Calibration

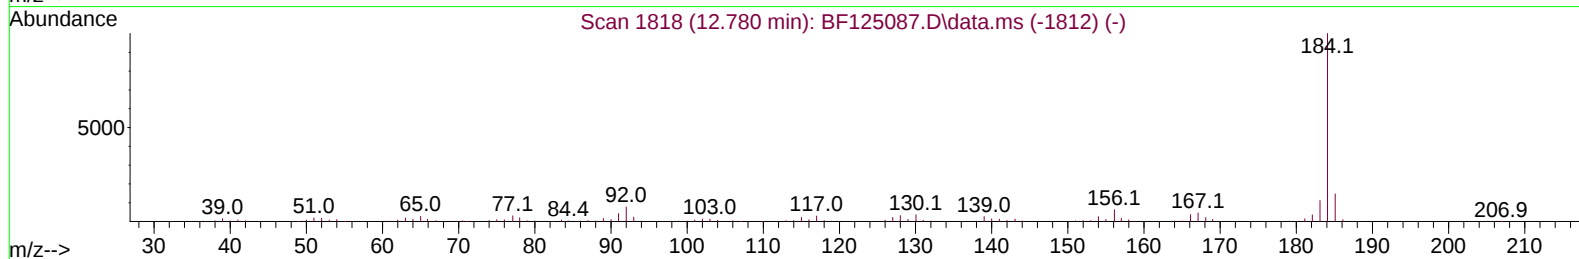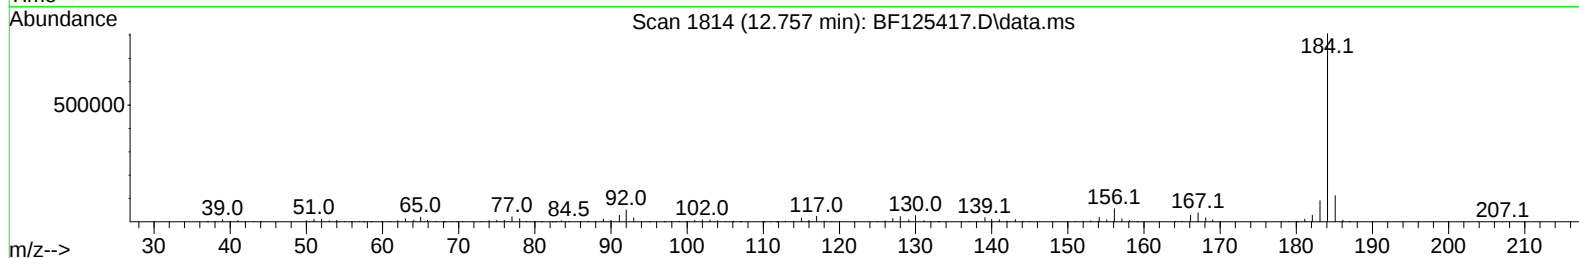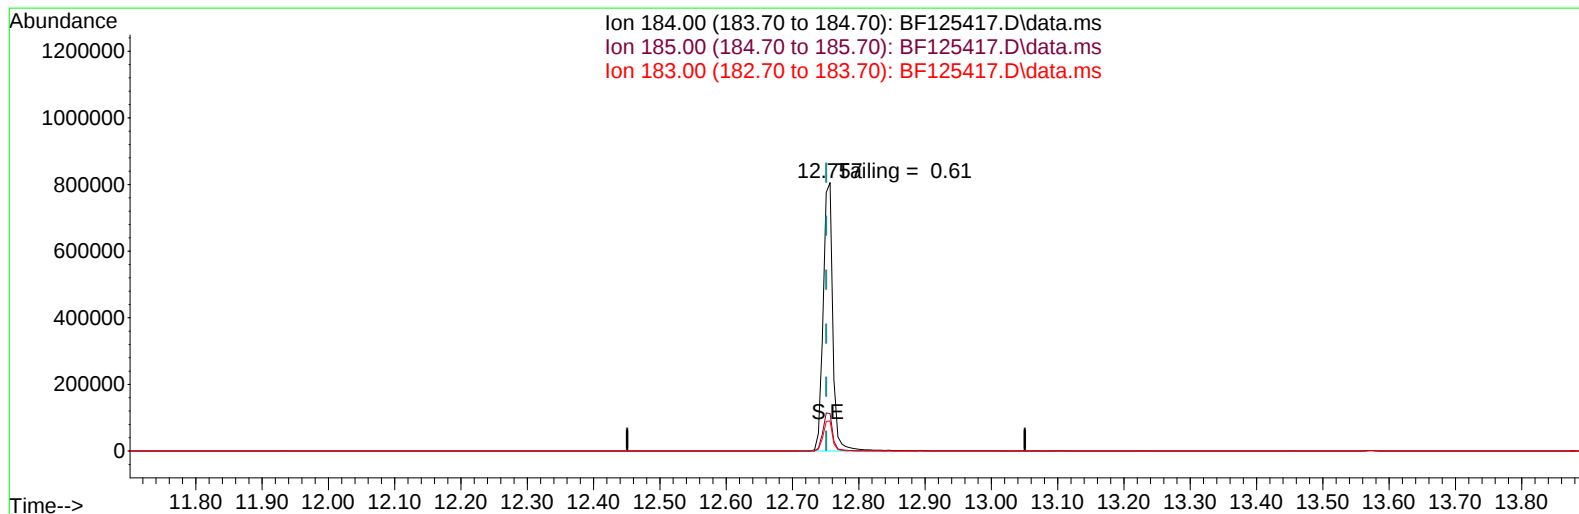

TIC: BF125417.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response 815789

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.94
183.00	10.10	11.24
0.00	0.00	0.00