
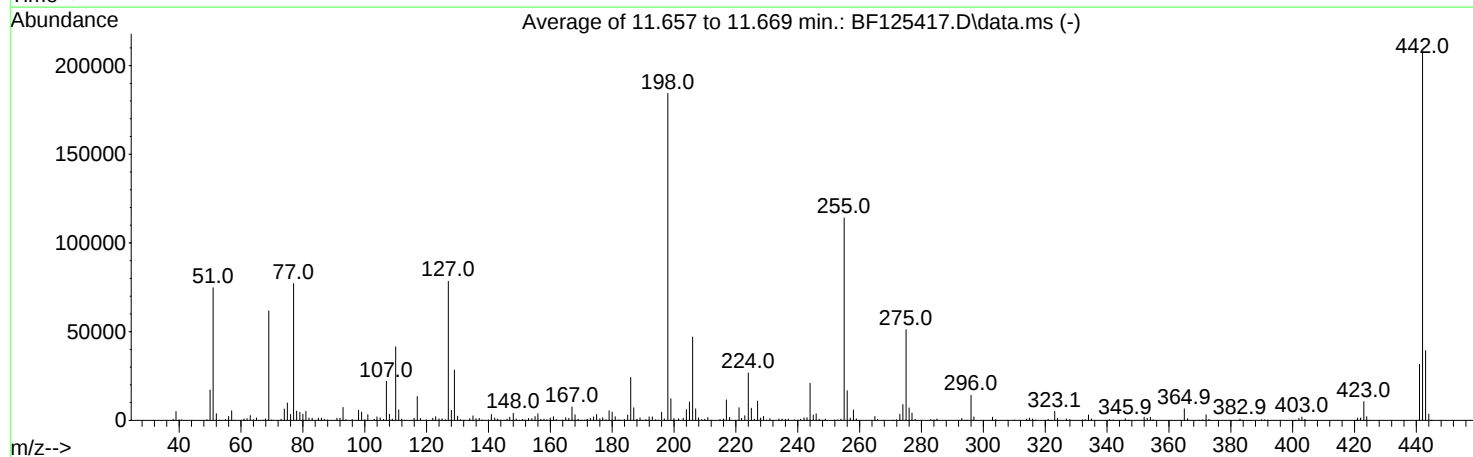


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091021\
 Data File : BF125417.D
 Acq On : 10 Sep 2021 10:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 08 14:14:01 2021

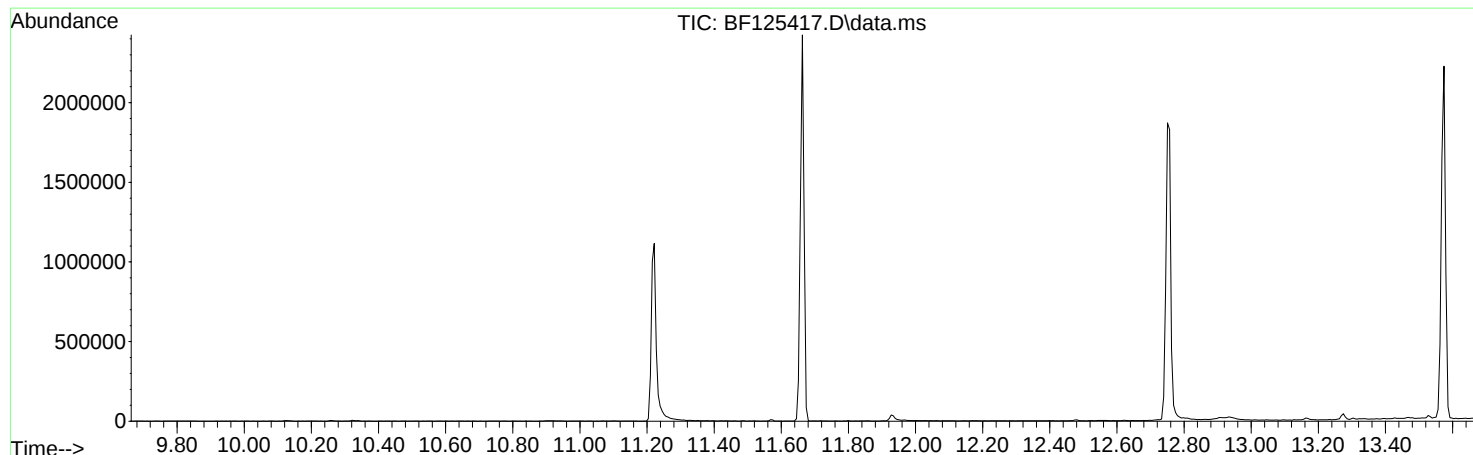

AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	74744	PASS
68	69	0.00	2	1.4	862	PASS
69	198	0.00	100	33.5	61667	PASS
70	69	0.00	2	0.4	253	PASS
127	198	10	80	42.5	78395	PASS
197	198	0.00	2	0.5	931	PASS
198	198	100	100	100.0	184333	PASS
199	198	5	9	6.6	12218	PASS
275	198	10	60	27.8	51173	PASS
365	198	1	100	3.5	6460	PASS
441	198	0.01	100	17.1	31568	PASS
442	442	50	100	100.0	207371	PASS
443	442	15	24	19.0	39309	PASS




DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/10/2021	BNA_F	<u>BF125417.D</u>
Compound Name	Response	Retention Time
DDT	393366	13.57
DDD	7510	13.27
DDE	1372	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8882	402248	2.21

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091021\
 Data File : BF125417.D
 Acq On : 10 Sep 2021 10:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 10 13:10:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 08 14:14:01 2021
 Response via : Initial Calibration

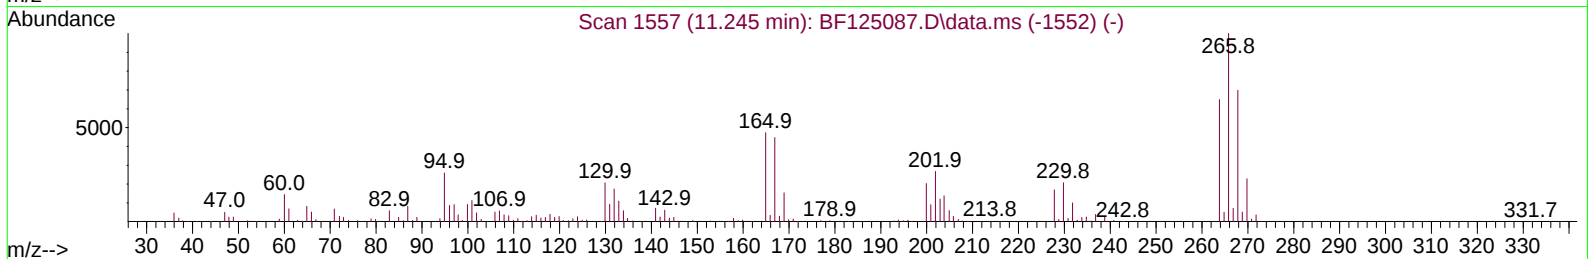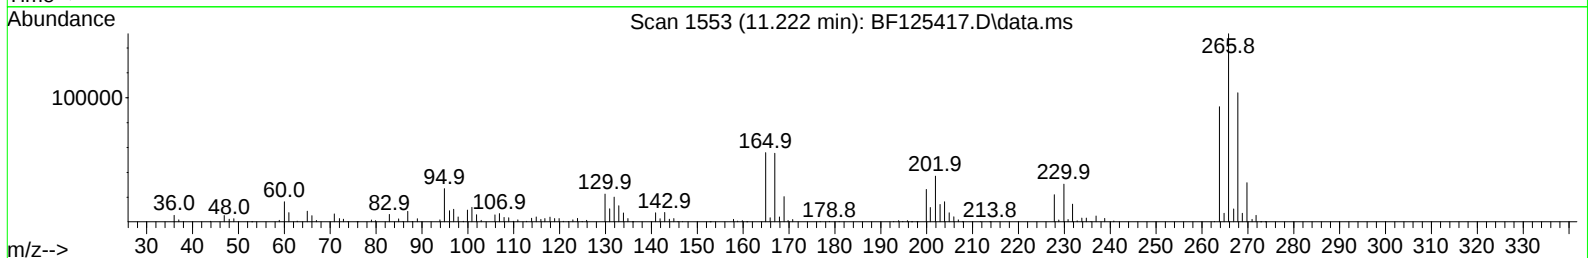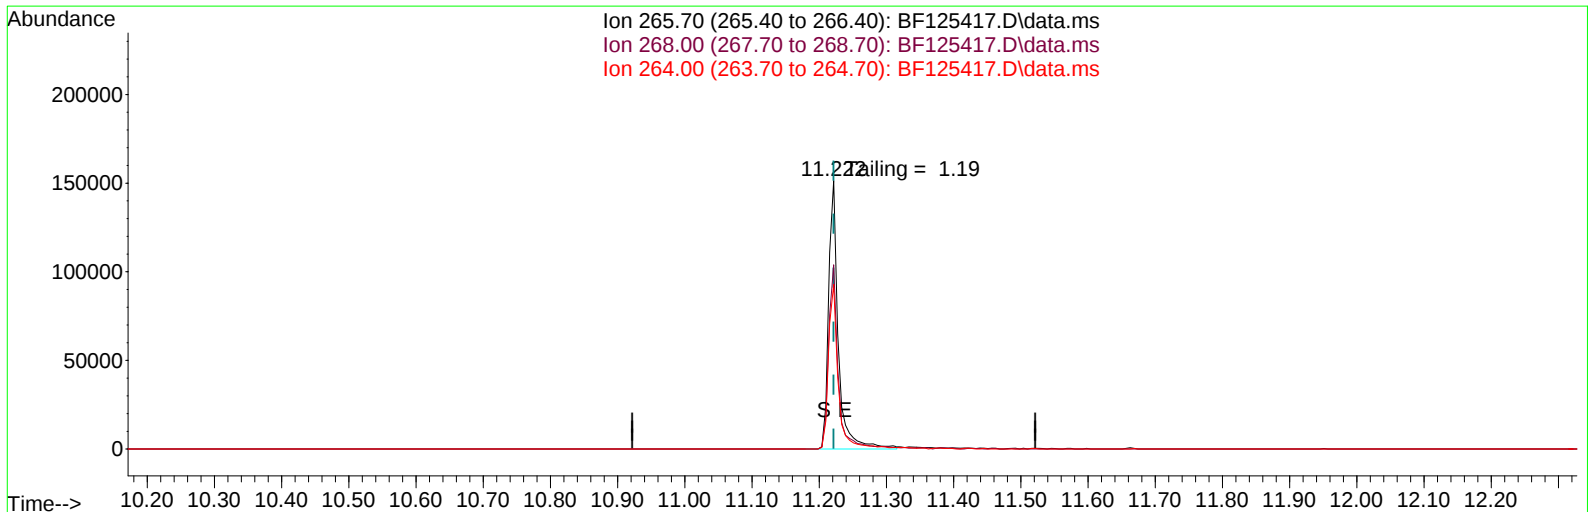

TIC: BF125417.D\data.ms

(70) Pentachlorophenol (C)

11.222min (+ 0.000) 26317.11 ng




response 153190

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	68.63
264.00	69.90	61.30
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091021\
 Data File : BF125417.D
 Acq On : 10 Sep 2021 10:11
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 10 13:10:55 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF081821.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 08 14:14:01 2021
 Response via : Initial Calibration

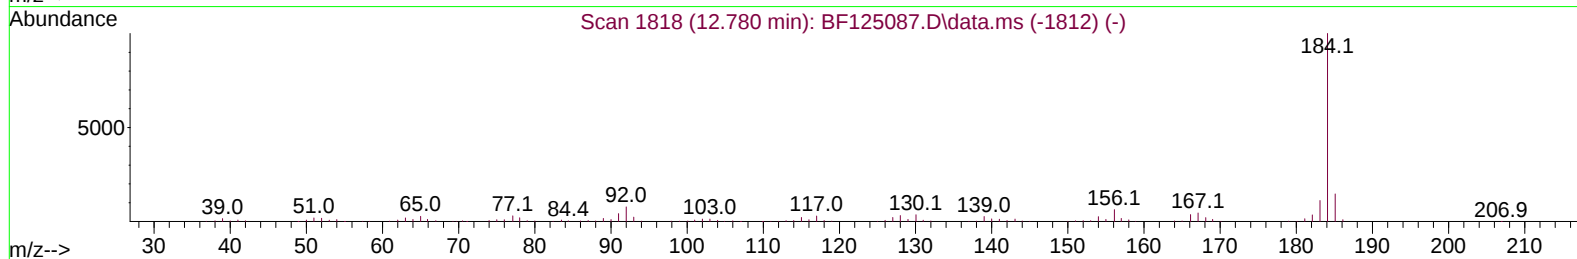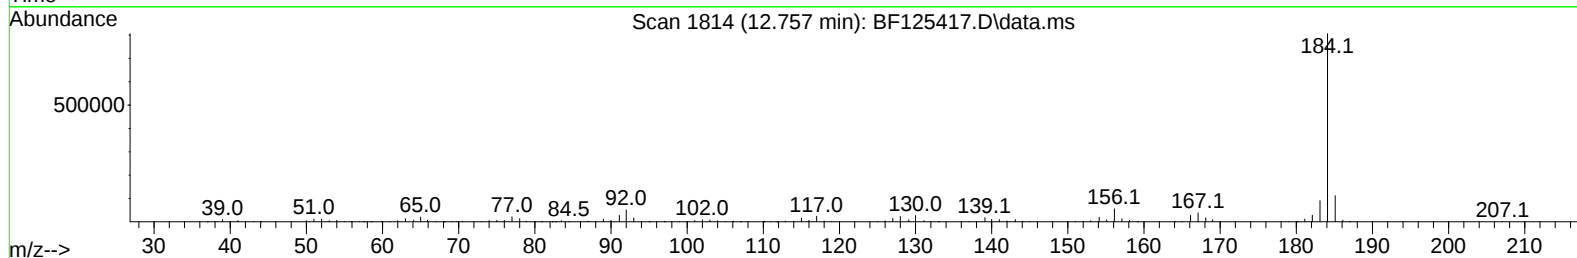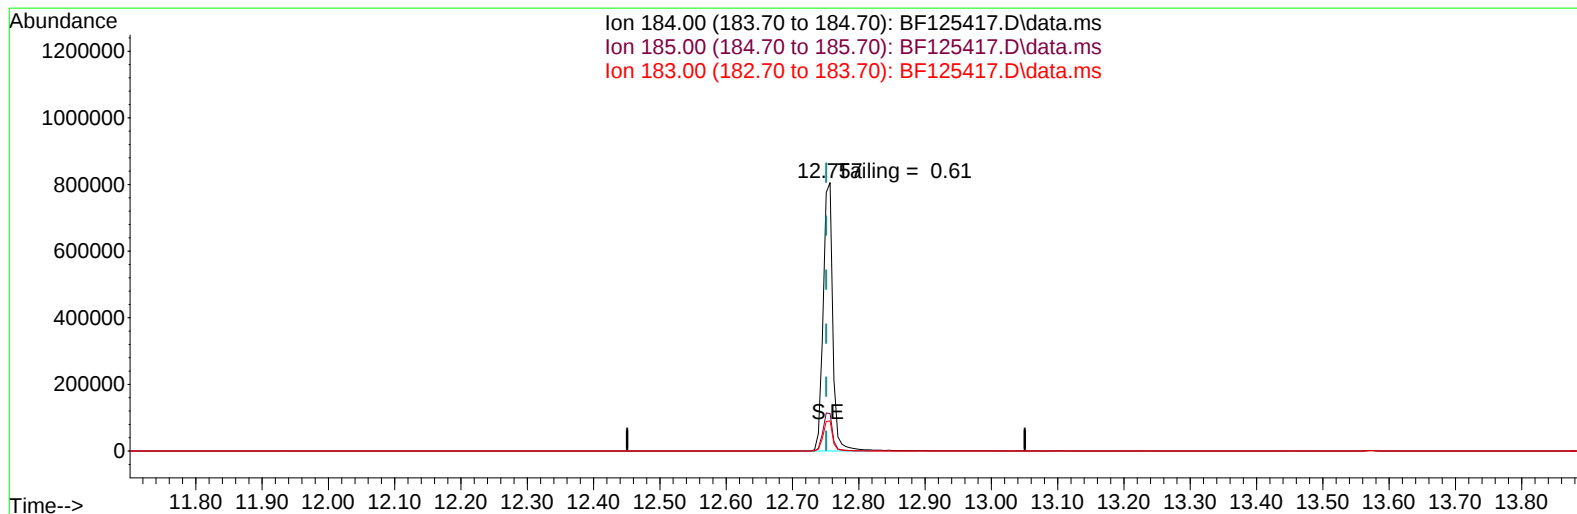

TIC: BF125417.D\data.ms

(77) Benzidine

12.757min (+ 0.006) 0.00 ng

response 815789

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.94
183.00	10.10	11.24
0.00	0.00	0.00