

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091024\
 Data File : BF139308.D
 Acq On : 10 Sep 2024 19:29
 Operator : RC/JU
 Sample : P3892-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 ARS20-005

Quant Time: Sep 11 01:31:22 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 04 16:11:43 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.887	152	114398	20.000	ng	0.00
21) Naphthalene-d8	8.169	136	418582	20.000	ng	0.00
39) Acenaphthene-d10	9.922	164	217865	20.000	ng	0.00
64) Phenanthrene-d10	11.410	188	329963	20.000	ng	0.00
76) Chrysene-d12	14.045	240	205914	20.000	ng	0.00
86) Perylene-d12	15.521	264	158592	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.516	112	742572	108.588	ng	0.01
7) Phenol-d6	6.516	99	918415	100.602	ng	0.00
23) Nitrobenzene-d5	7.451	82	697182	86.648	ng	0.00
42) 2,4,6-Tribromophenol	10.716	330	249800	132.781	ng	0.00
45) 2-Fluorobiphenyl	9.245	172	1294916	91.749	ng	0.00
79) Terphenyl-d14	12.998	244	1185154	92.928	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091024\
Data File : BF139308.D
Acq On : 10 Sep 2024 19:29
Operator : RC/JU
Sample : P3892-02
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
ARS20-005

Quant Time: Sep 11 01:31:22 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration




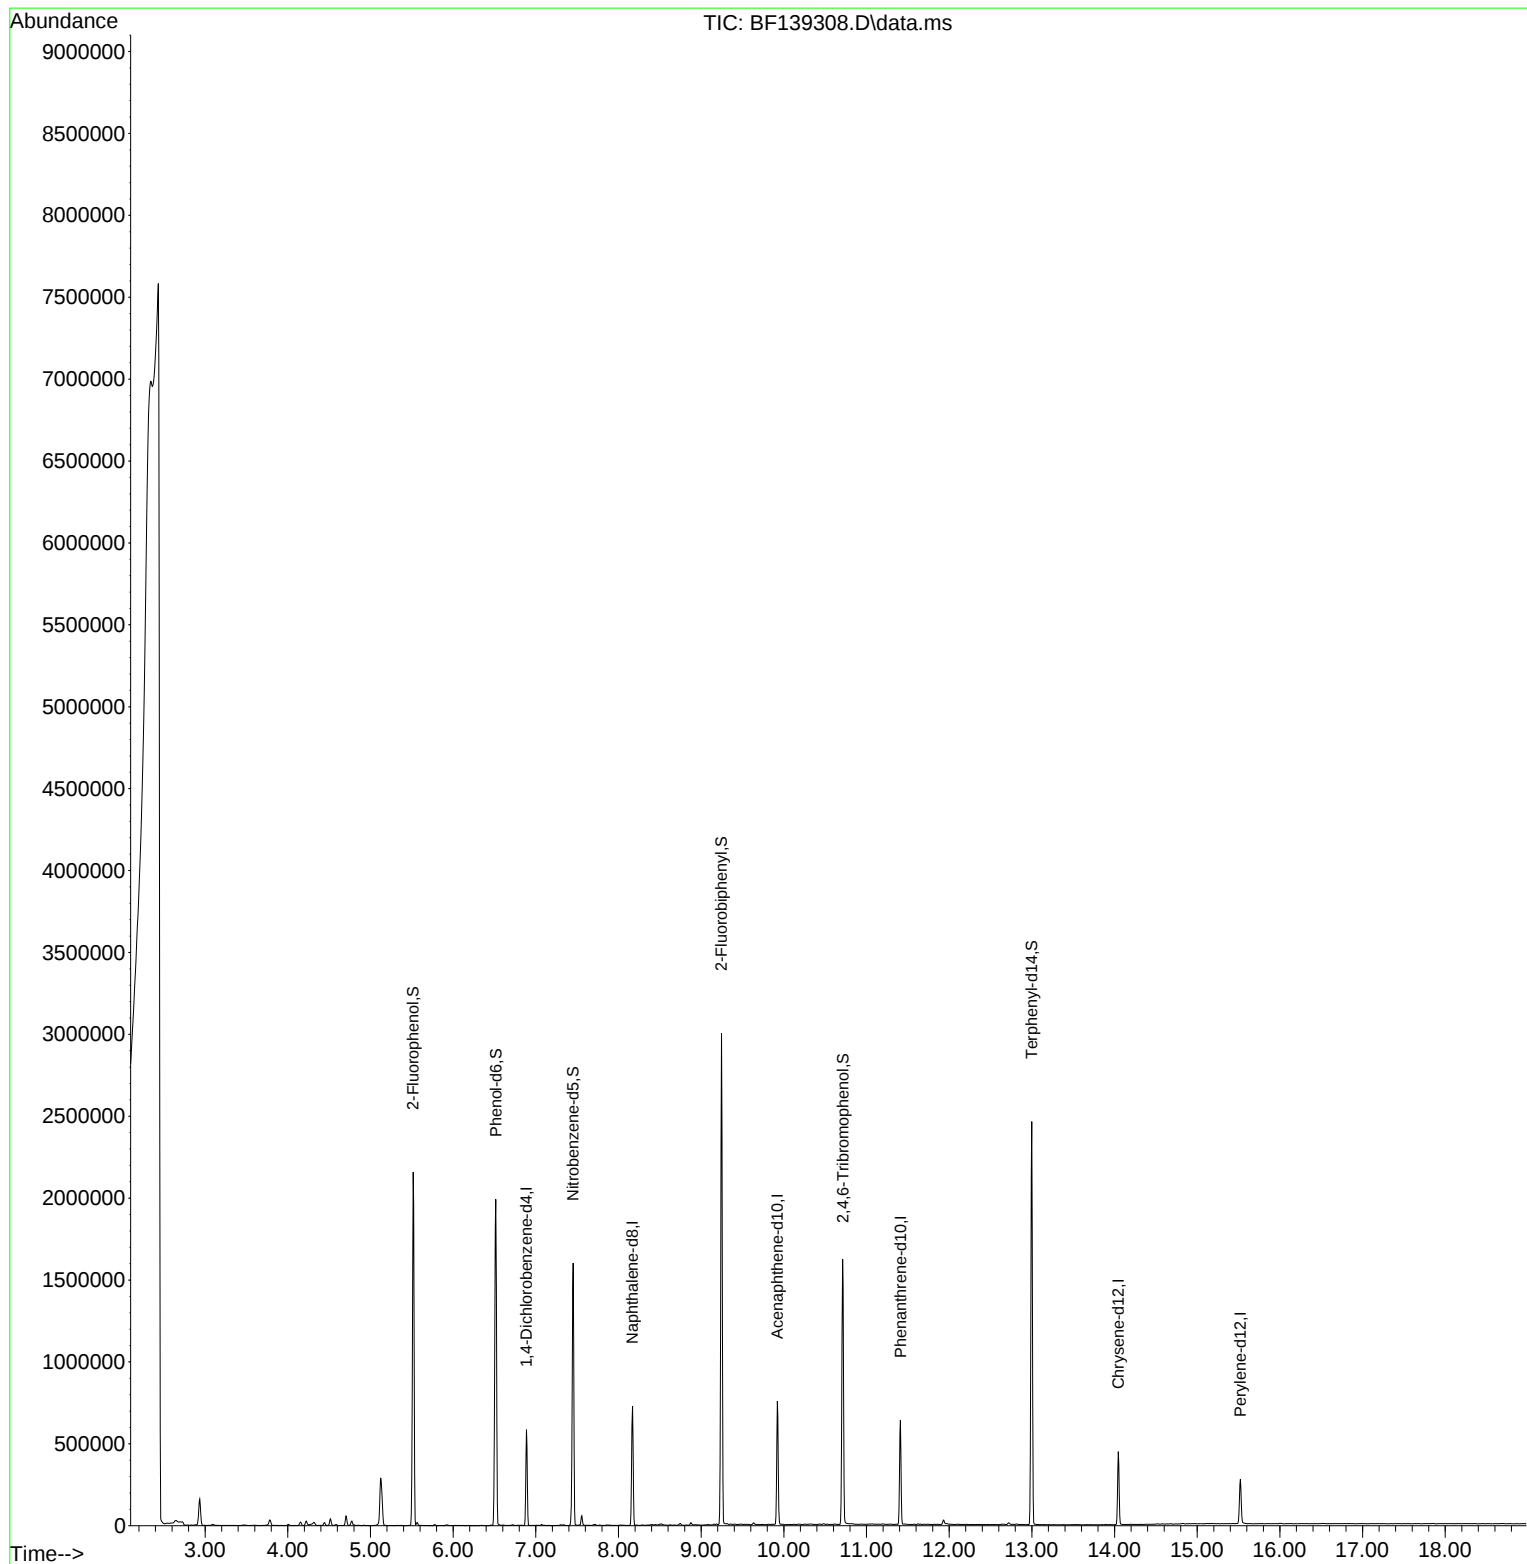


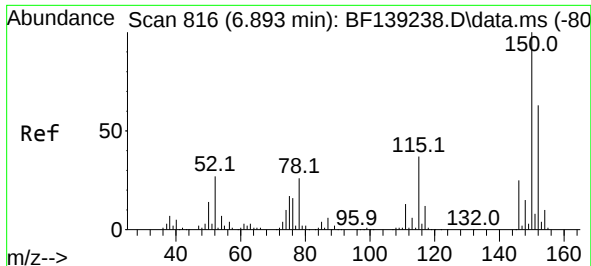

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.887 min Scan# 816
Delta R.T. -0.006 min
Lab File: BF139308.D
Acq: 10 Sep 2024 19:29




Instrument :
BNA_F
ClientSampleId :
ARS20-005

Tgt Ion:152 Resp: 114398
Ion Ratio Lower Upper
152 100
150 155.9 127.0 190.4
115 60.8 46.9 70.3

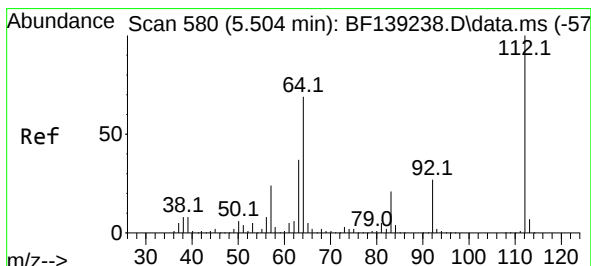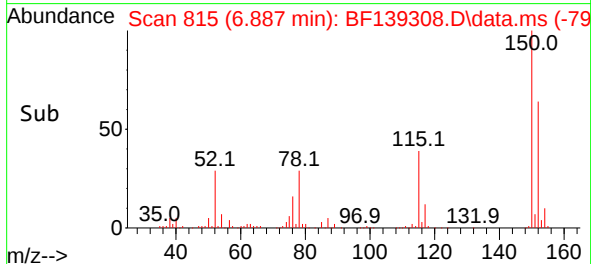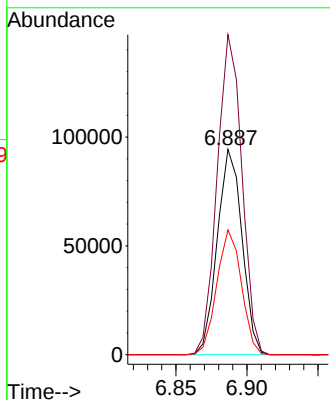

#5
2-Fluorophenol
Concen: 108.588 ng
RT: 5.516 min Scan# 582
Delta R.T. 0.012 min
Lab File: BF139308.D
Acq: 10 Sep 2024 19:29

Tgt Ion:112 Resp: 742572
Ion Ratio Lower Upper
112 100
64 70.2 55.0 82.4
63 38.3 29.9 44.9

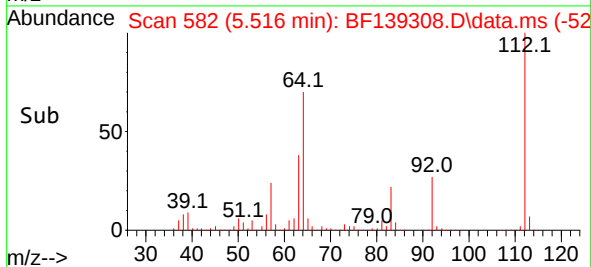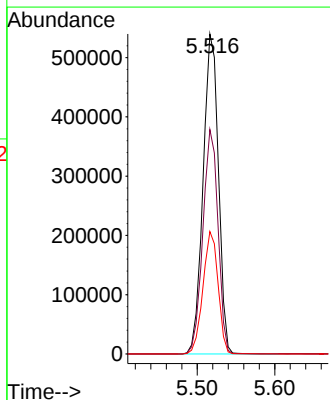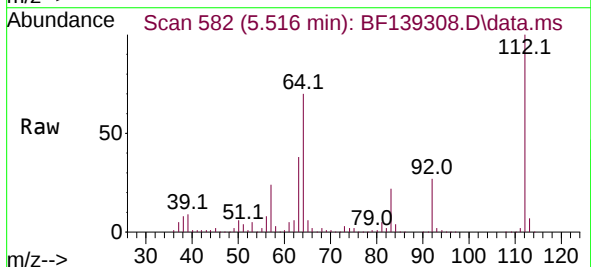



#7

Phenol-d6

Concen: 100.602 ng

RT: 6.516 min Scan# 71

Delta R.T. -0.000 min

Lab File: BF139308.D

Acq: 10 Sep 2024 19:29

Instrument :

BNA_F

ClientSampleId :

ARS20-005





Tgt Ion: 99 Resp: 918415

Ion Ratio Lower Upper

99 100

42 23.6 19.8 29.6

71 36.9 28.8 43.2

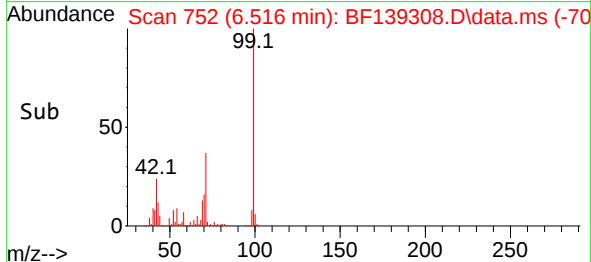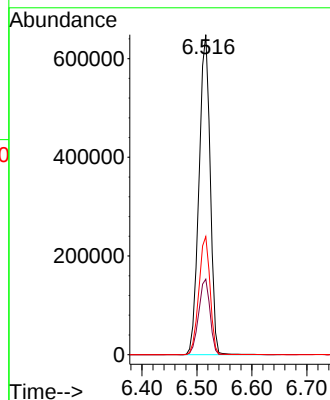

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.169 min Scan# 1033

Delta R.T. -0.006 min

Lab File: BF139308.D

Acq: 10 Sep 2024 19:29

Tgt Ion:136 Resp: 418582




Ion Ratio Lower Upper


136 100

137 10.9 8.6 13.0

54 10.1 8.4 12.6

68 6.1 4.8 7.2


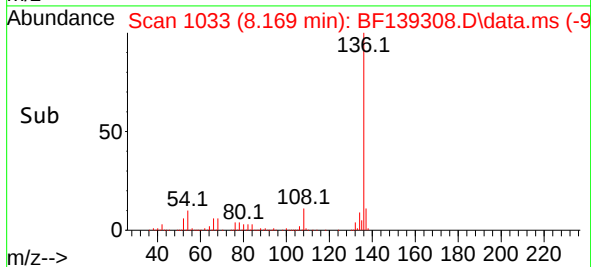
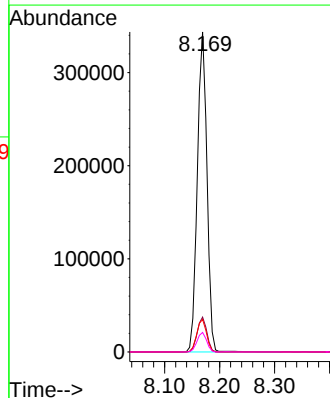
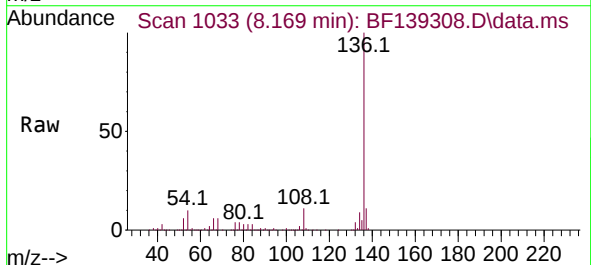


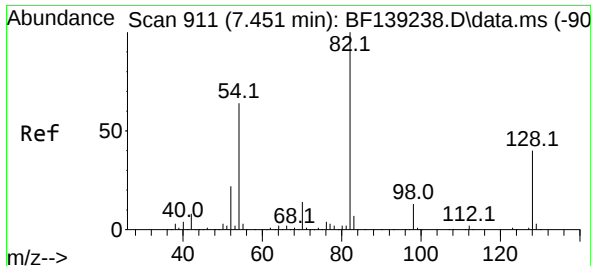

#23
Nitrobenzene-d5
Concen: 86.648 ng
RT: 7.451 min Scan# 911
Delta R.T. -0.000 min
Lab File: BF139308.D
Acq: 10 Sep 2024 19:29




Instrument :
BNA_F
ClientSampleId :
ARS20-005


Tgt Ion: 82 Resp: 697182
Ion Ratio Lower Upper
82 100
128 41.9 32.3 48.5
54 61.1 51.2 76.8

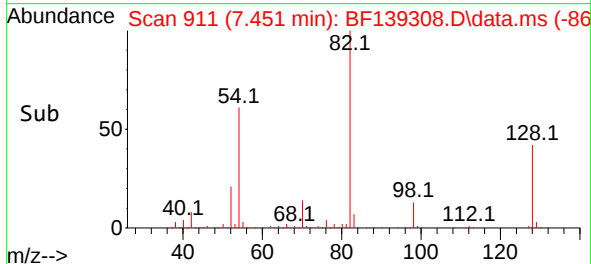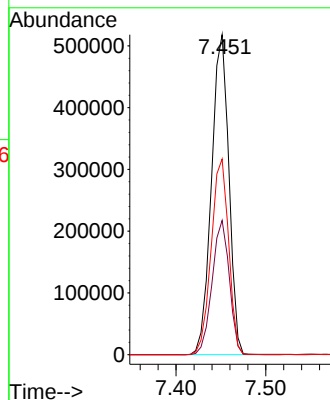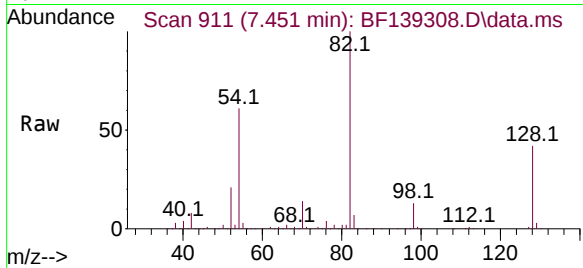

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.922 min Scan# 1331
Delta R.T. -0.006 min
Lab File: BF139308.D
Acq: 10 Sep 2024 19:29


Tgt Ion:164 Resp: 217865
Ion Ratio Lower Upper
164 100
162 98.4 79.2 118.8
160 44.1 34.2 51.2

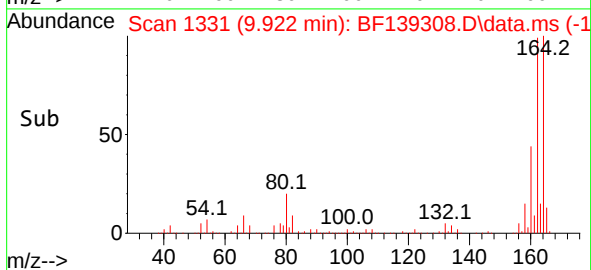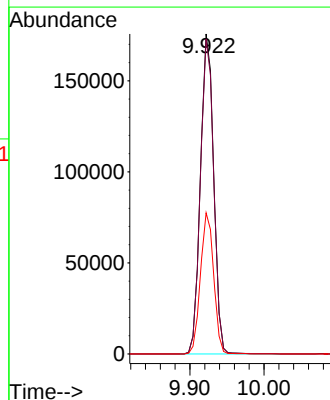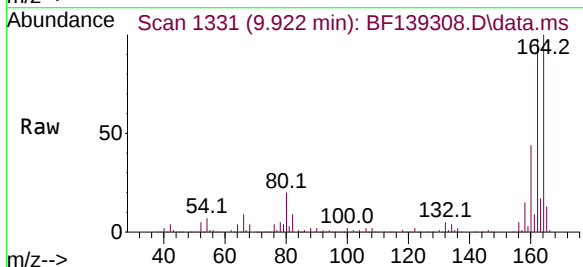



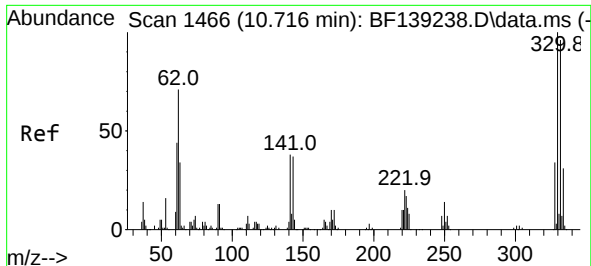


#42
2,4,6-Tribromophenol
Concen: 132.781 ng
RT: 10.716 min Scan# 1466
Delta R.T. -0.000 min
Lab File: BF139308.D
Acq: 10 Sep 2024 19:29


Instrument :
BNA_F
ClientSampleId :
ARS20-005

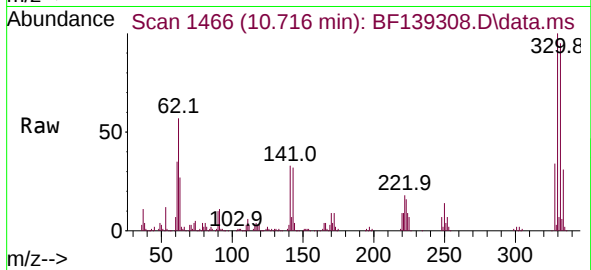



Tgt Ion:330 Resp: 249800
Ion Ratio Lower Upper
330 100
332 94.7 76.6 115.0
141 36.5 30.1 45.1

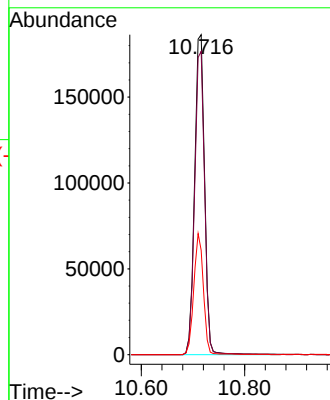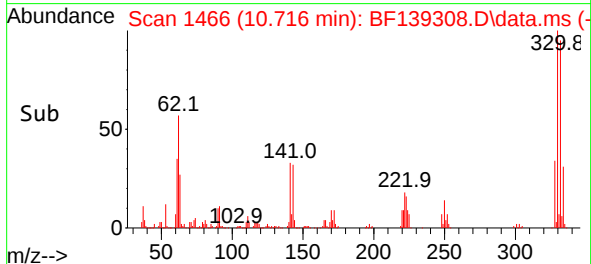


#45
2-Fluorobiphenyl
Concen: 91.749 ng
RT: 9.245 min Scan# 1216
Delta R.T. -0.006 min
Lab File: BF139308.D
Acq: 10 Sep 2024 19:29

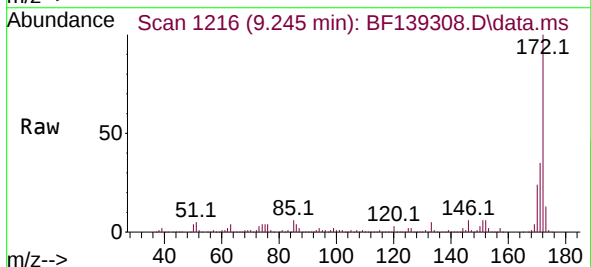

Tgt Ion:172 Resp: 1294916
Ion Ratio Lower Upper
172 100
171 35.4 28.3 42.5
170 23.6 18.7 28.1

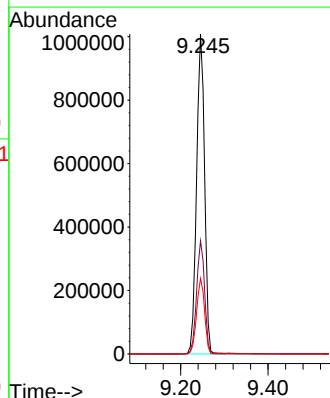



#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.410 min Scan# 11

Delta R.T. -0.006 min

Lab File: BF139308.D

Acq: 10 Sep 2024 19:29

Instrument :

BNA_F

ClientSampleId :

ARS20-005





Tgt Ion:188 Resp: 329963

Ion Ratio Lower Upper

188 100

94 8.4 7.0 10.4

80 9.5 7.3 10.9

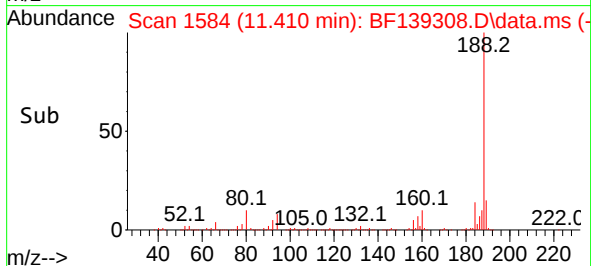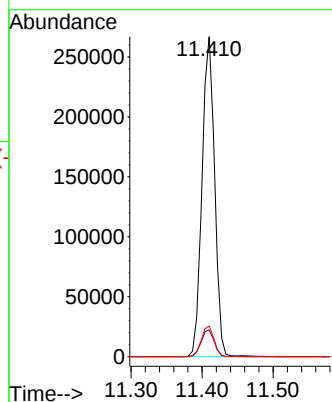

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.045 min Scan# 2032

Delta R.T. -0.006 min

Lab File: BF139308.D

Acq: 10 Sep 2024 19:29




Tgt Ion:240 Resp: 205914


Ion Ratio Lower Upper

240 100

120 9.7 8.6 12.8

236 26.1 20.7 31.1


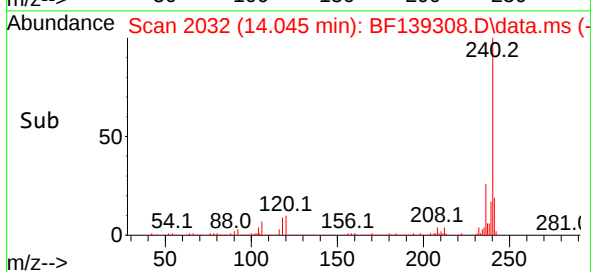
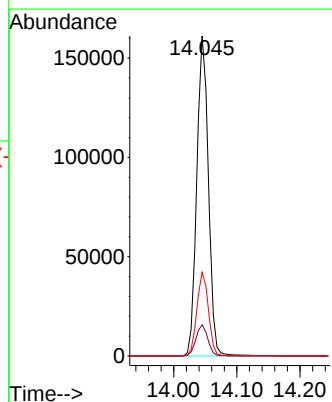
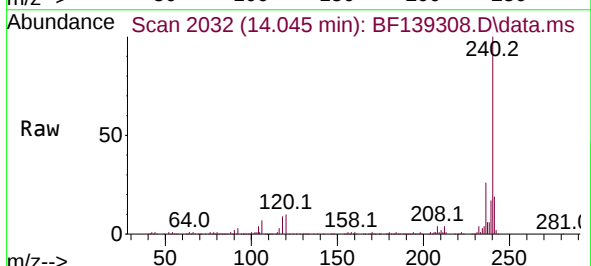


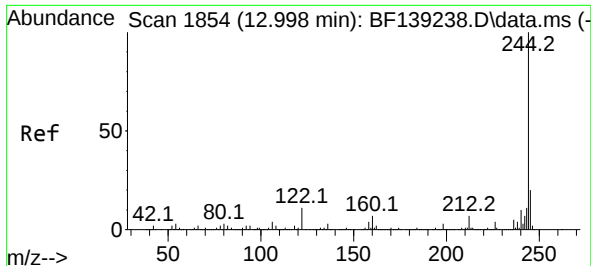

#79
 Terphenyl-d14
 Concen: 92.928 ng
 RT: 12.998 min Scan# 11
 Delta R.T. -0.000 min
 Lab File: BF139308.D
 Acq: 10 Sep 2024 19:29

Instrument :
 BNA_F
 ClientSampleId :
 ARS20-005

Tgt Ion:244 Resp: 1185154
 Ion Ratio Lower Upper
 244 100
 212 7.3 5.9 8.9
 122 10.3 8.7 13.1

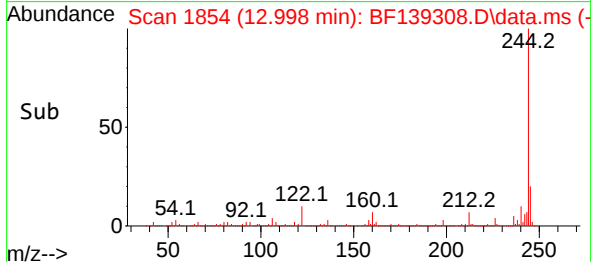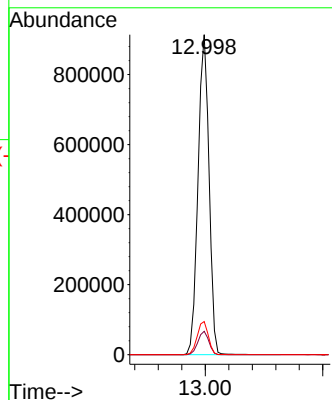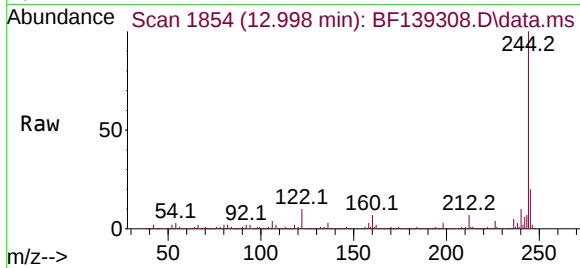

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.521 min Scan# 2283
 Delta R.T. -0.006 min
 Lab File: BF139308.D
 Acq: 10 Sep 2024 19:29

Tgt Ion:264 Resp: 158592
 Ion Ratio Lower Upper
 264 100
 260 22.9 18.8 28.2
 265 21.7 17.3 25.9

