


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091024\
Data File : BF139292.D
Acq On : 10 Sep 2024 11:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 04 16:11:43 2024

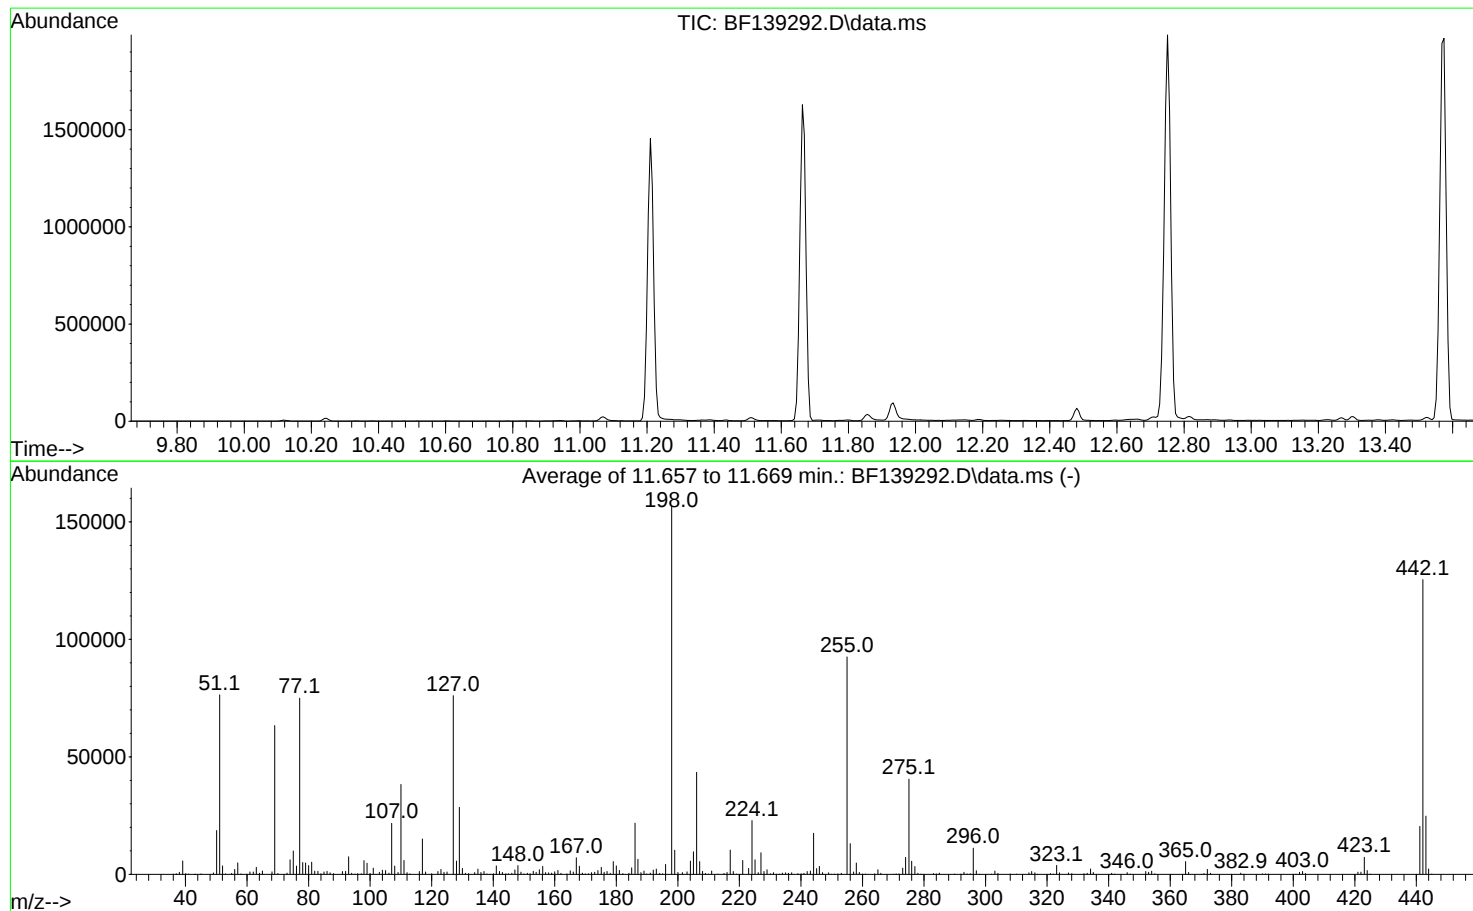

AutoFind: Scans 1626, 1627, 1628; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	76400	PASS
68	69	0.00	2	1.7	1089	PASS
69	198	0.00	100	40.4	63303	PASS
70	69	0.00	2	0.6	403	PASS
127	198	10	80	48.6	76043	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	156552	PASS
199	198	5	9	6.6	10304	PASS
275	198	10	60	25.9	40499	PASS
365	198	1	100	3.5	5426	PASS
441	198	0.01	100	13.1	20465	PASS
442	442	50	100	100.0	125435	PASS
443	442	15	24	19.8	24801	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/10/2024	BNA_F	<u>BF139292.D</u>
Compound Name	Response	Retention Time
DDT	504606	13.574
DDD	8923	13.304
DDE	386	12.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9309	513915	1.81

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091024\
Data File : BF139292.D
Acq On : 10 Sep 2024 11:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 10 11:49:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

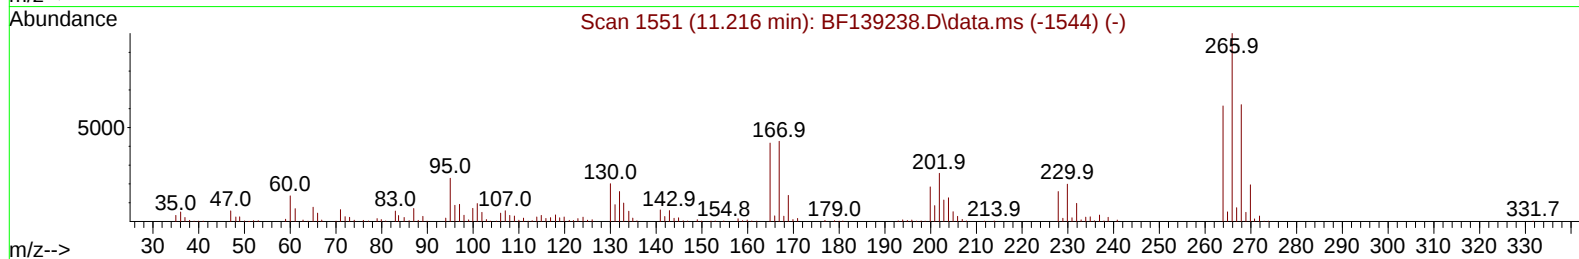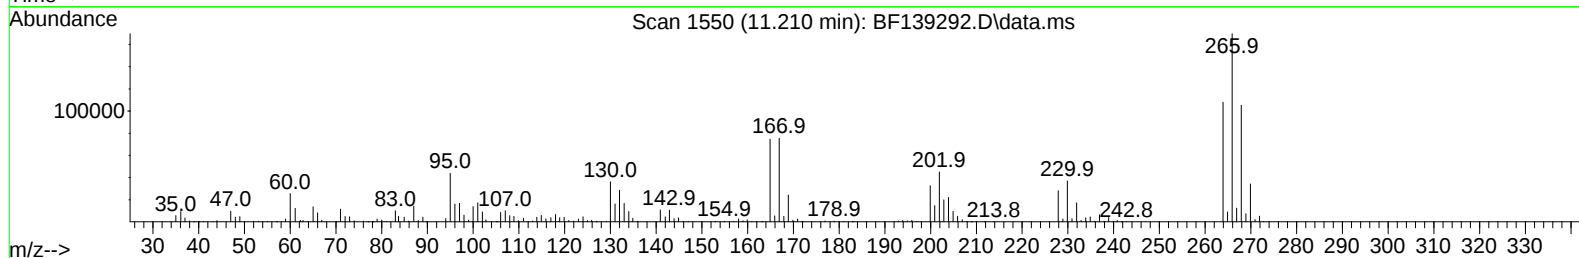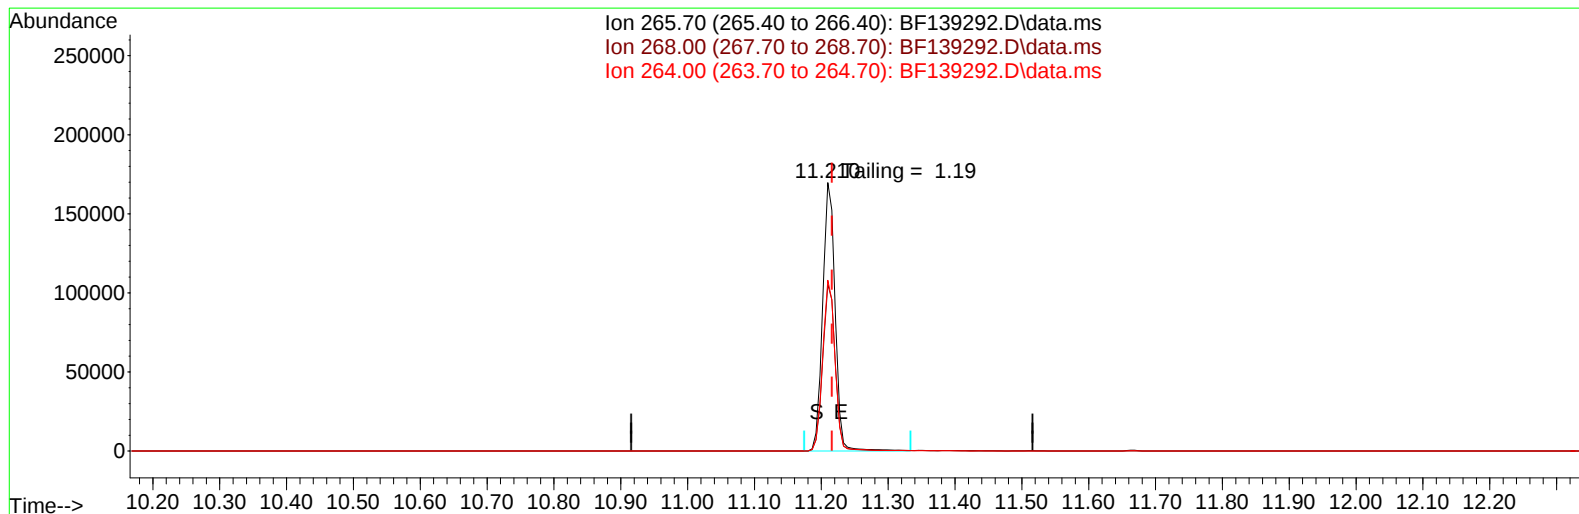

TIC: BF139292.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 33421.33 ng




response 220649

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	62.03
264.00	61.50	63.63
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091024\
Data File : BF139292.D
Acq On : 10 Sep 2024 11:00
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 10 11:49:15 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

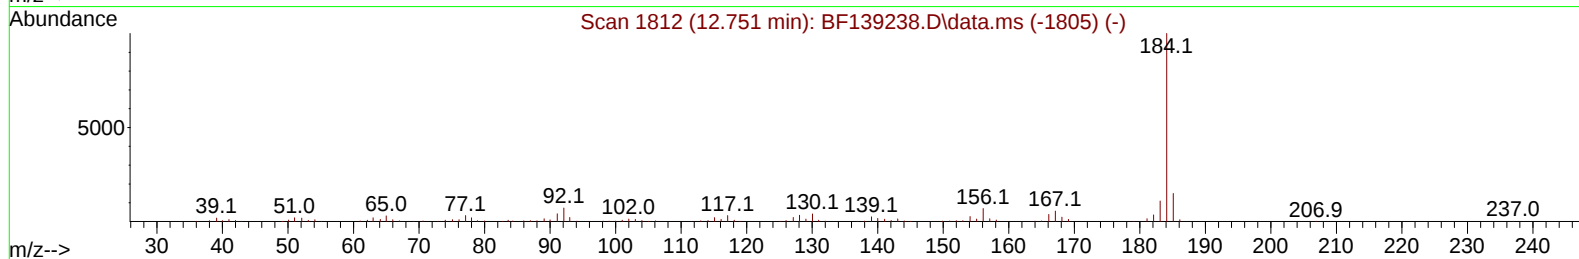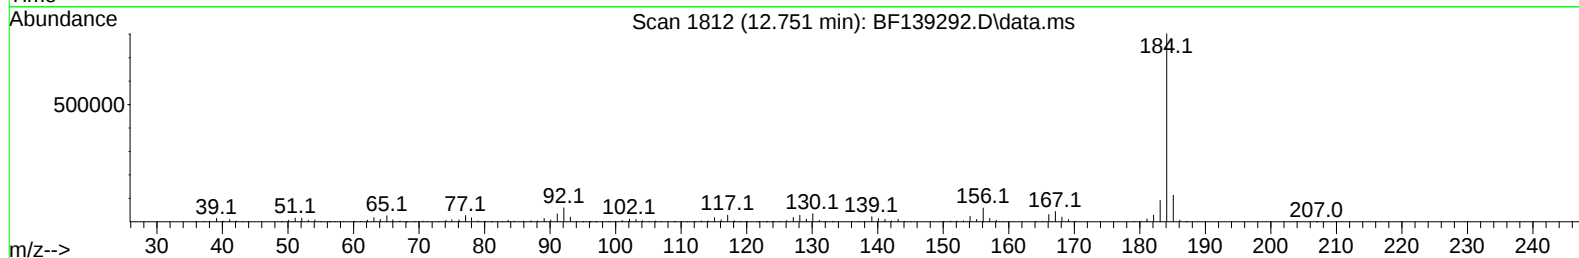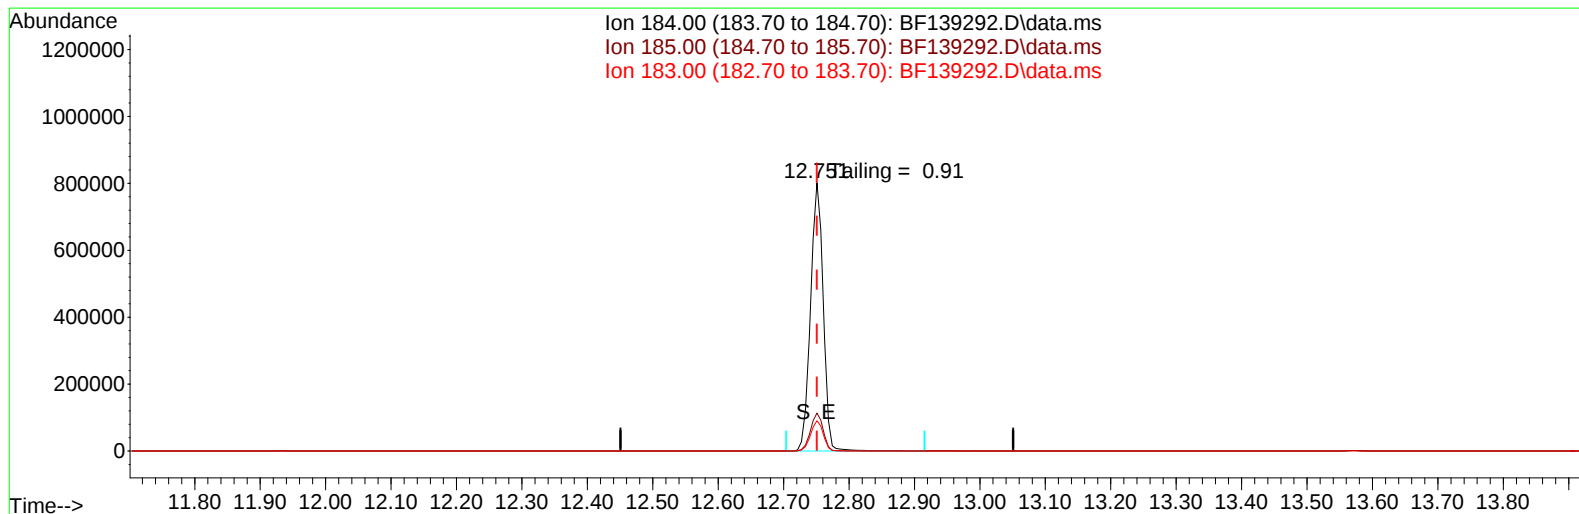

TIC: BF139292.D\data.ms

(77) Benzidine

12.751min (-0.000) 0.00 ng

response 1084291

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.14
183.00	11.00	11.31
0.00	0.00	0.00