


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091025\
Data File : BF143692.D
Acq On : 10 Sep 2025 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 09 15:20:16 2025

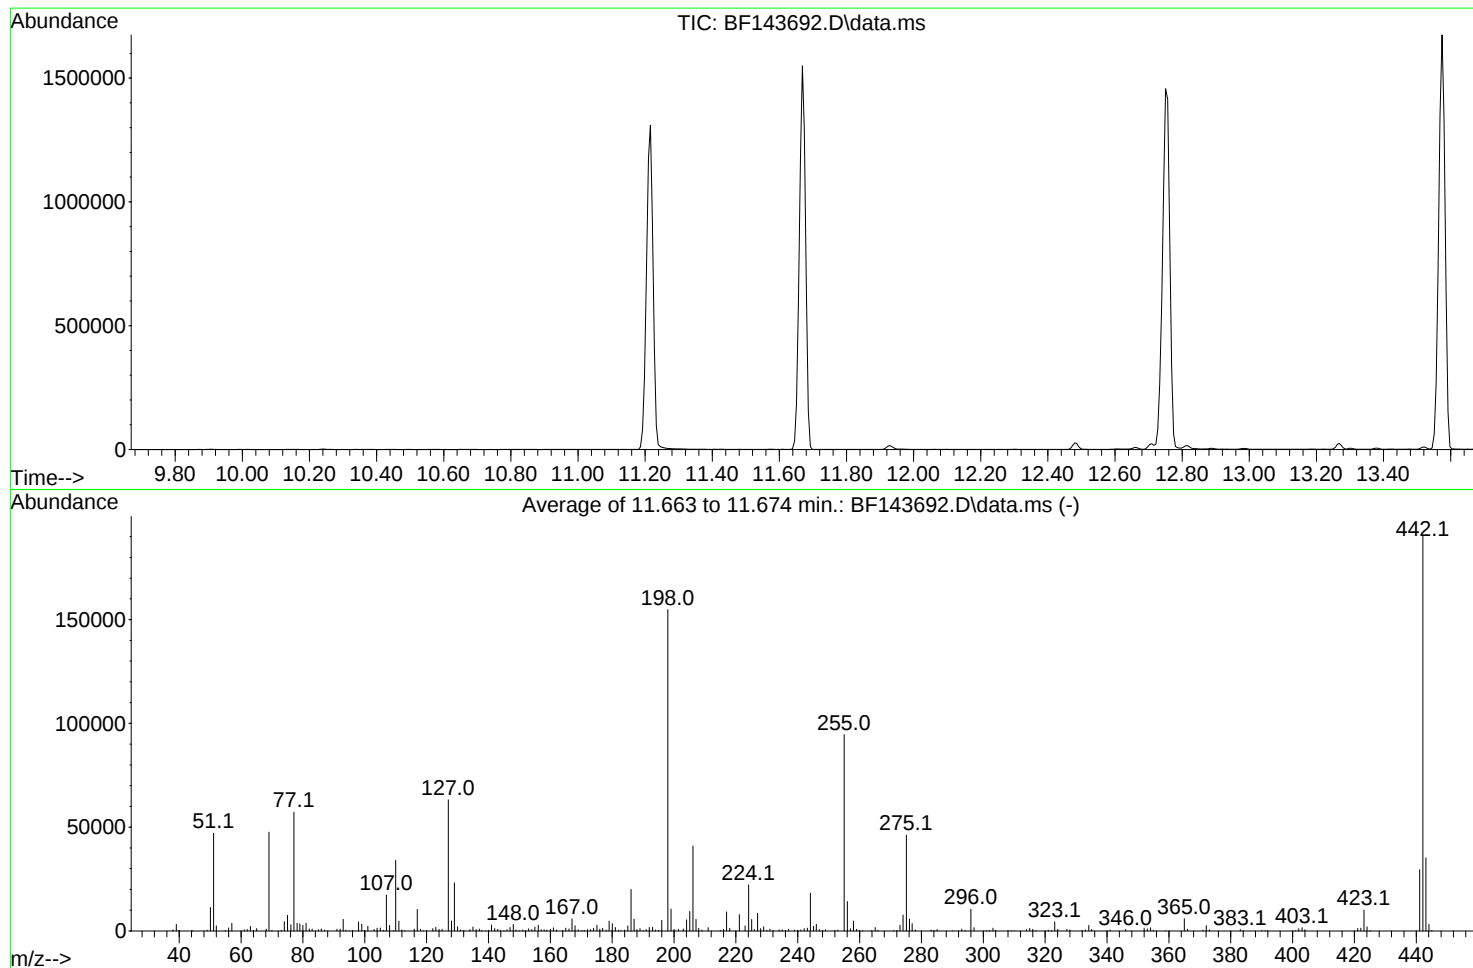

AutoFind: Scans 1610, 1611, 1612; Background Corrected with Scan 1603

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	926	PASS
69	69	100	100	100.0	47581	PASS
70	69	0.00	2	0.6	276	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	154880	PASS
199	198	5	9	6.8	10519	PASS
365	198	1	100	3.8	5927	PASS
441	443	0.01	150	83.8	29477	PASS
442	442	100	100	100.0	190251	PASS
443	442	15	24	18.5	35168	PASS