
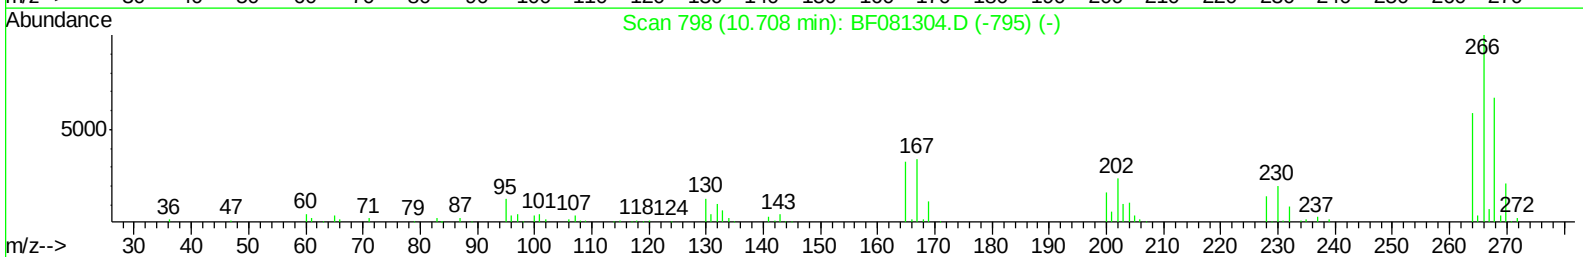
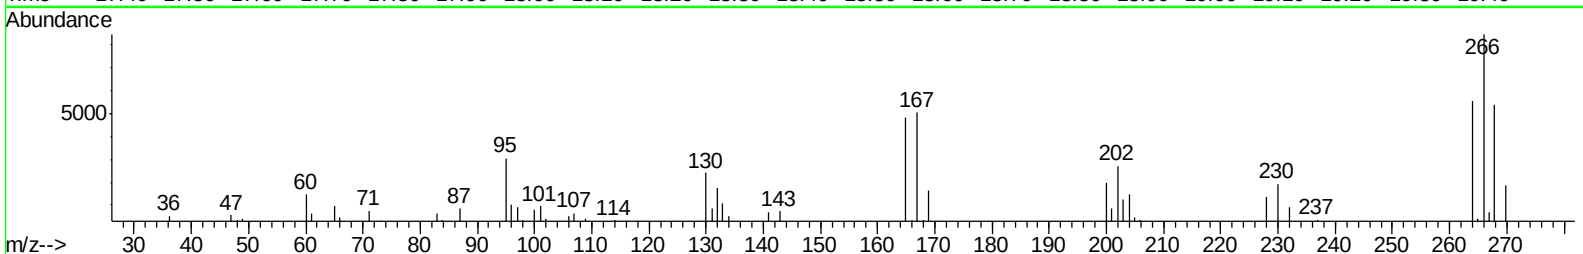


Data Path : Z:\HPCHEM1\BNA_F\Data\BF091115\
Data File : BF081584.D
Acq On : 11 Sep 2015 14:37
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 03:32:54 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 10 16:31:29 2015
Response via : Initial Calibration

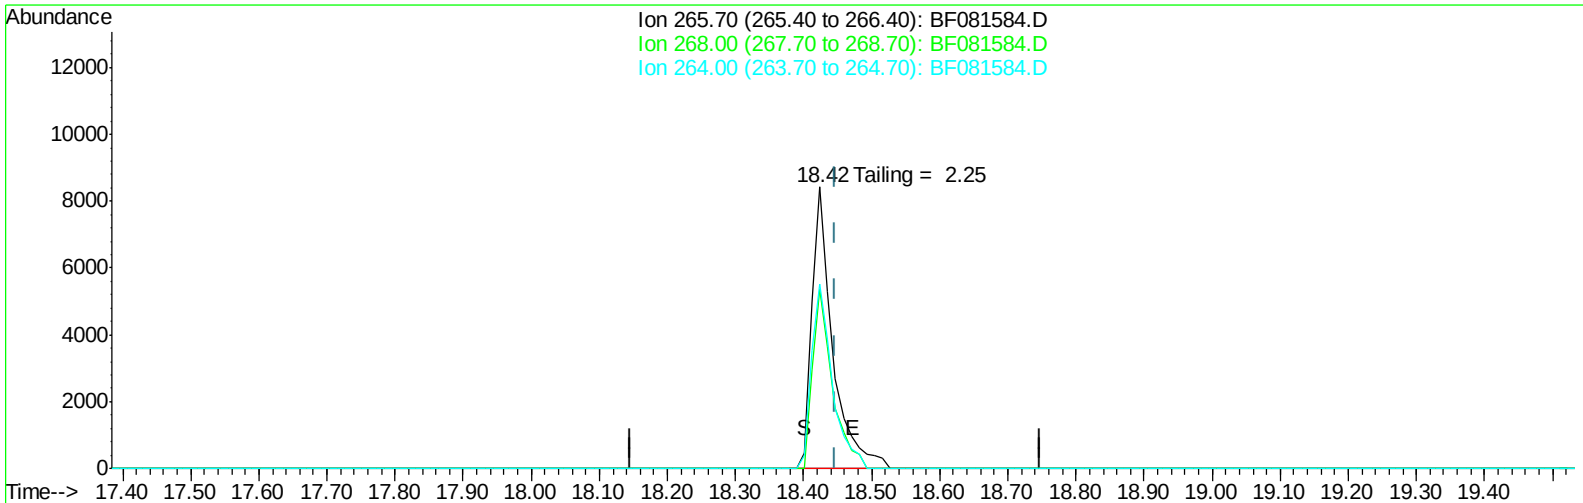

TIC: BF081584.D

(69) Pentachlorophenol (C)




18.424min (-0.023) 0.00ng m

response 17854

Ion	Exp%	Act%
265.70	100	100
268.00	62.20	63.65
264.00	62.70	65.42
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF091115\
Data File : BF081584.D
Acq On : 11 Sep 2015 14:37
Operator : UM/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 03:32:54 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 10 16:31:29 2015
Response via : Initial Calibration

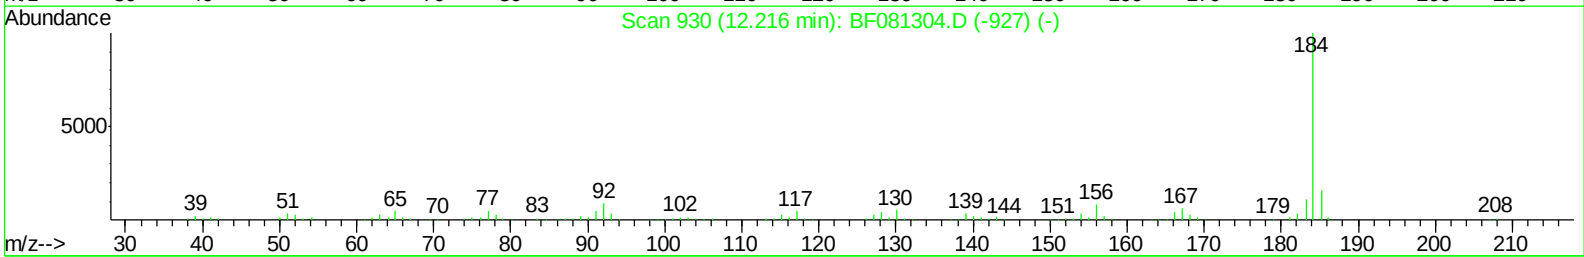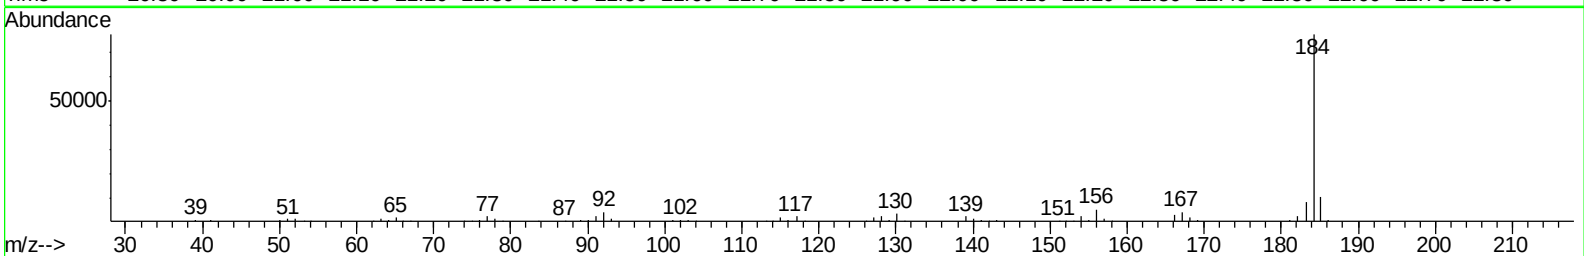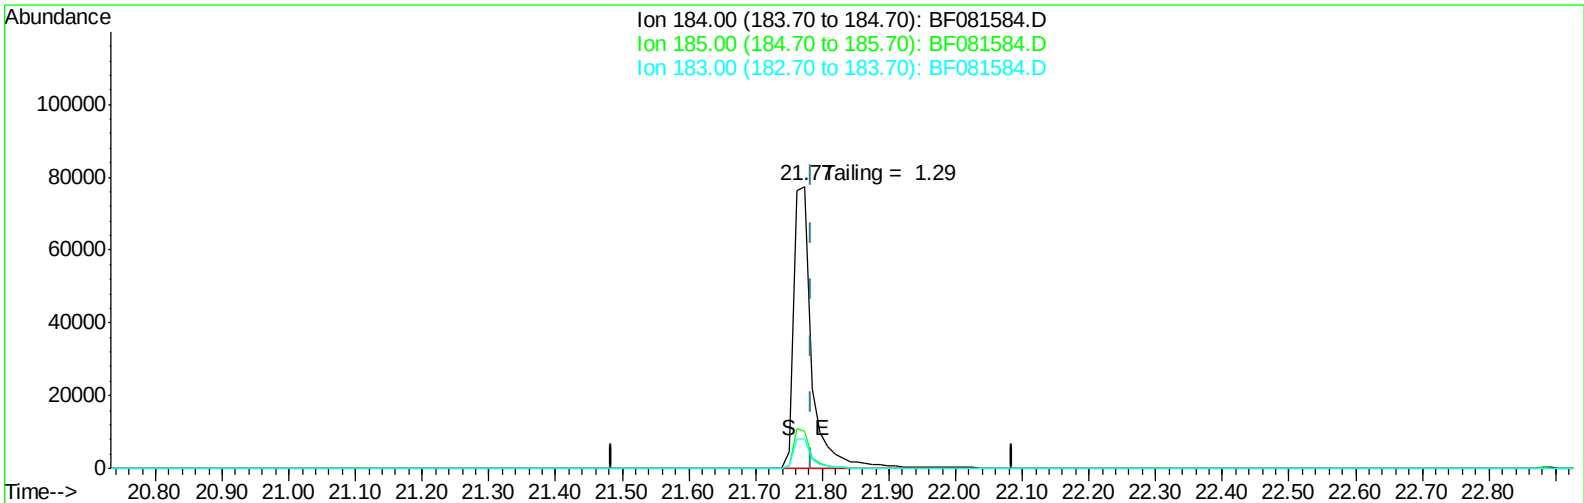

TIC: BF081584.D

(76) Benzidine

21.773min (-0.012) 0.00ng m

response 145270

Ion	Exp%	Act%
184.00	100	100
185.00	14.70	13.27
183.00	9.50	10.68
0.00	0.00	0.00