


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091115\
 Data File : BF081584.D
 Acq On : 11 Sep 2015 14:37
 Operator : UM/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF090115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 10 16:31:29 2015

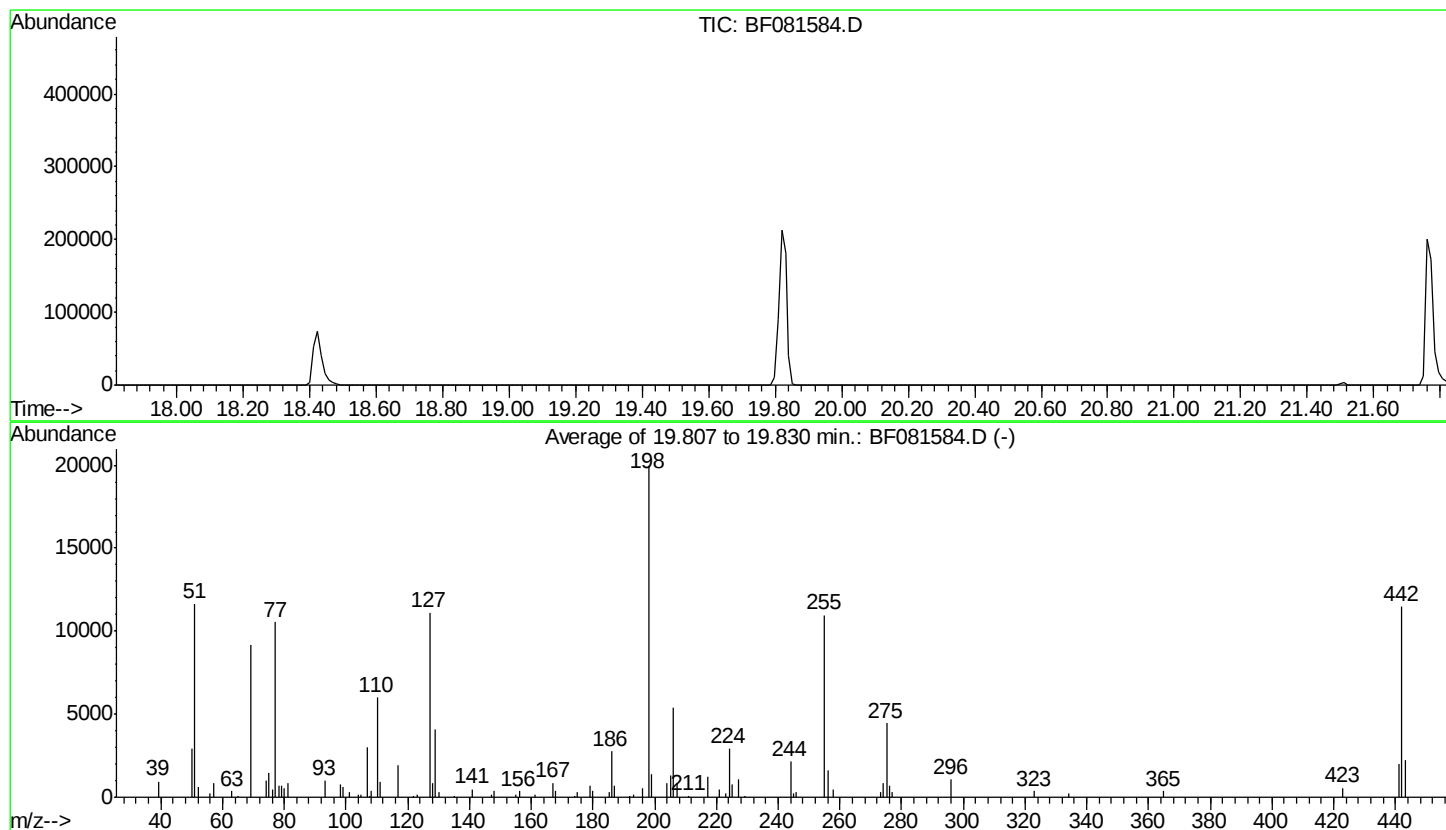

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.3	11648	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.1	9198	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.6	11108	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19972	PASS
199	198	5	9	6.8	1363	PASS
275	198	10	60	22.3	4455	PASS
365	198	1	100	1.8	364	PASS
441	442	0.01	24	17.7	2030	PASS
442	198	50	100	57.5	11487	PASS
443	442	15	24	19.3	2213	PASS