


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF091117\
 Data File : BF098437.D
 Acq On : 12 Sep 2017 7:55
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 02:14:50 2017

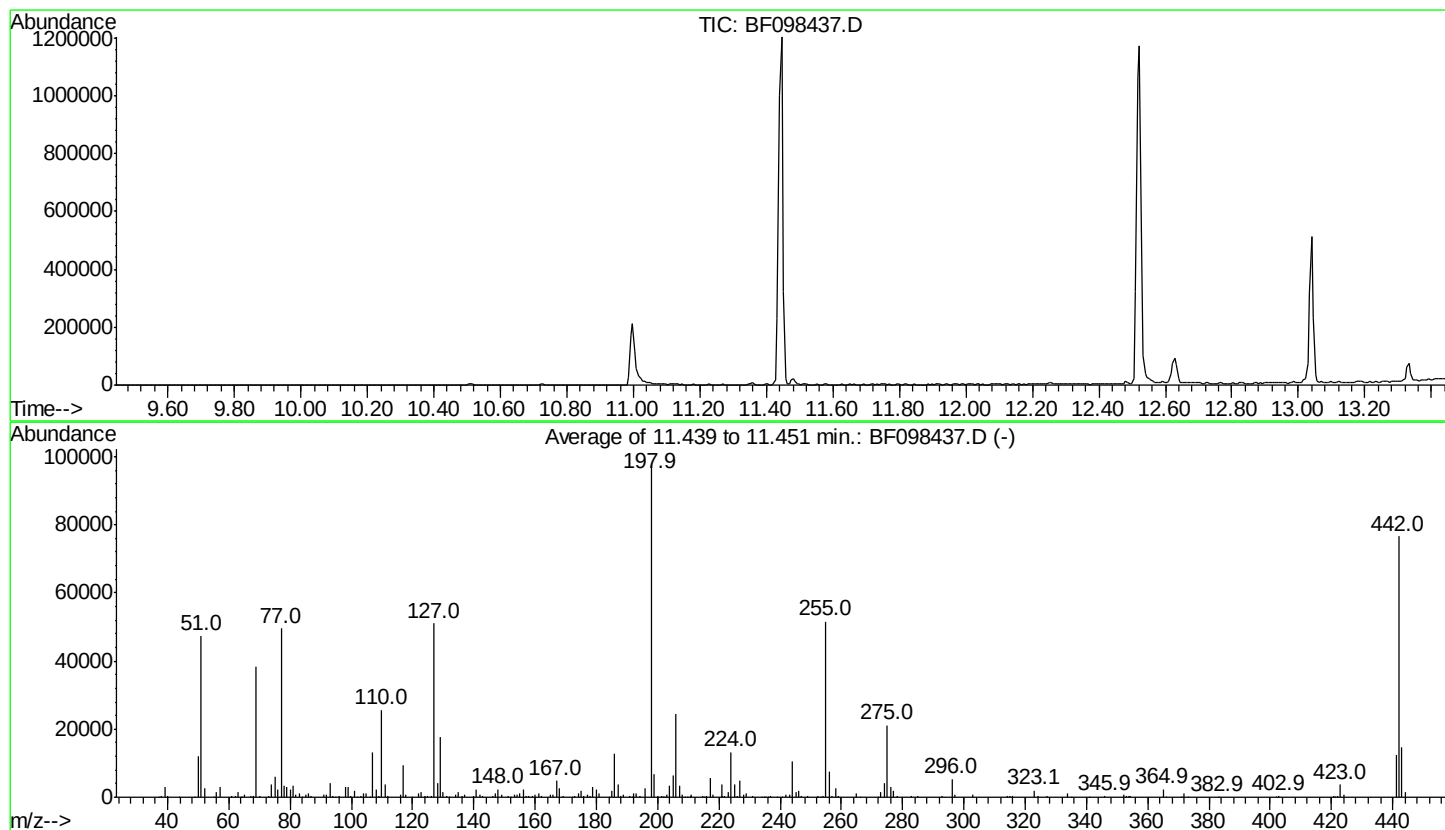

AutoFind: Scans 1590, 1591, 1592; Background Corrected with Scan 1585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	47471	PASS
68	69	0.00	2	1.0	392	PASS
69	198	0.00	100	39.6	38506	PASS
70	69	0.00	2	0.6	220	PASS
127	198	10	80	52.4	51056	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	97360	PASS
199	198	5	9	6.9	6747	PASS
275	198	10	60	21.8	21202	PASS
365	198	1	100	2.4	2338	PASS
441	442	0.01	24	16.0	12279	PASS
442	198	50	100	78.6	76546	PASS
443	442	15	24	18.9	14490	PASS