


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091124\
Data File : BF139314.D
Acq On : 11 Sep 2024 09:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 04 16:11:43 2024

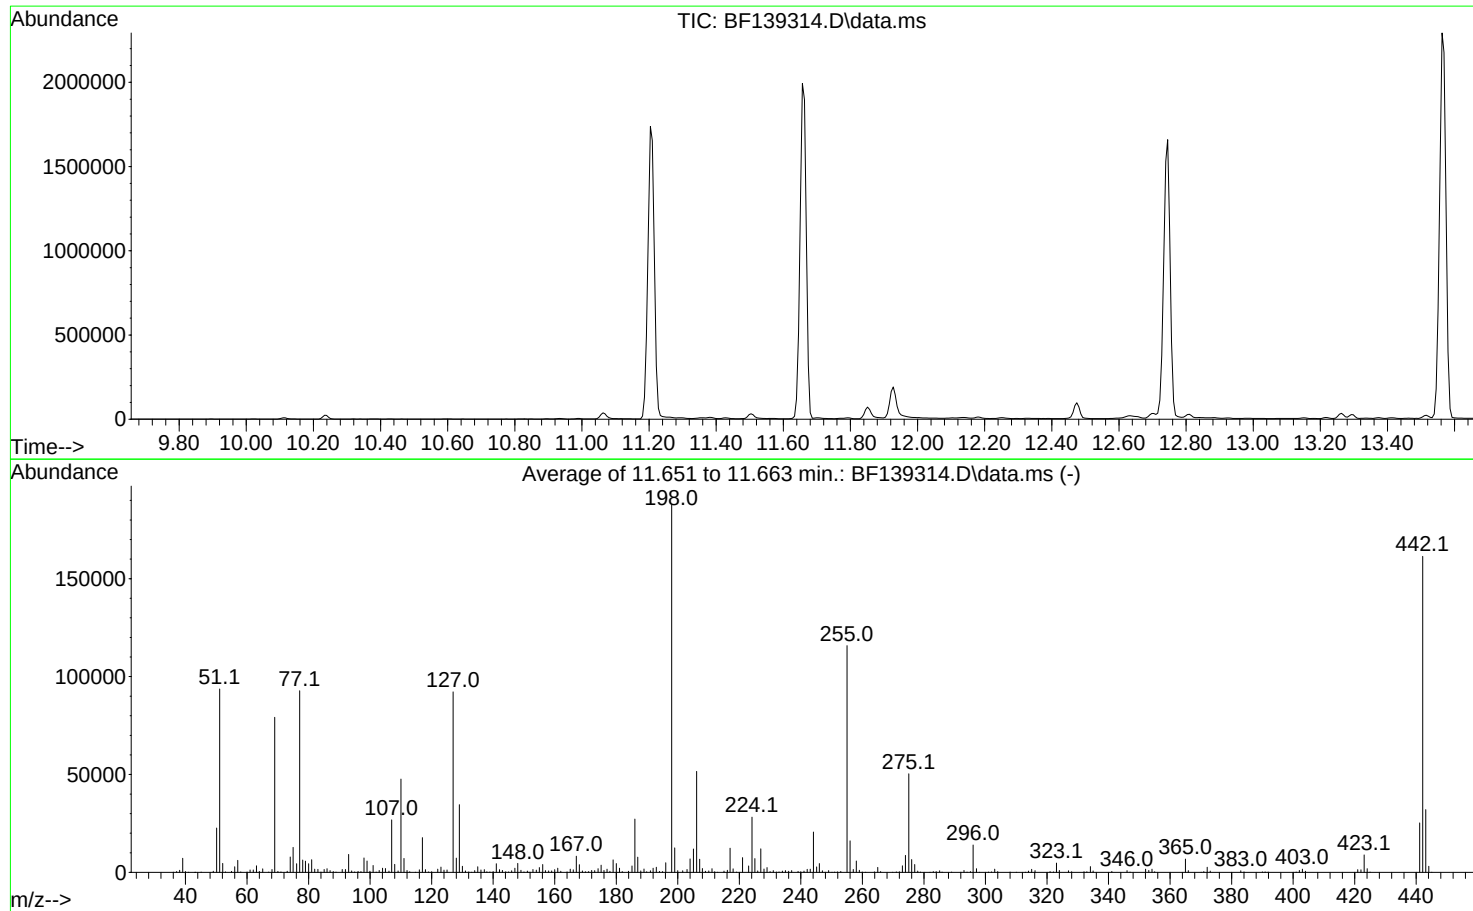




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.9	93677	PASS
68	69	0.00	2	1.9	1473	PASS
69	198	0.00	100	42.1	79185	PASS
70	69	0.00	2	0.6	502	PASS
127	198	10	80	49.0	92163	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	187904	PASS
199	198	5	9	6.7	12548	PASS
275	198	10	60	26.8	50355	PASS
365	198	1	100	3.6	6828	PASS
441	198	0.01	100	13.5	25300	PASS
442	442	50	100	100.0	161440	PASS
443	442	15	24	19.8	32035	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091124\
Data File : BF139314.D
Acq On : 11 Sep 2024 09:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 11 11:06:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

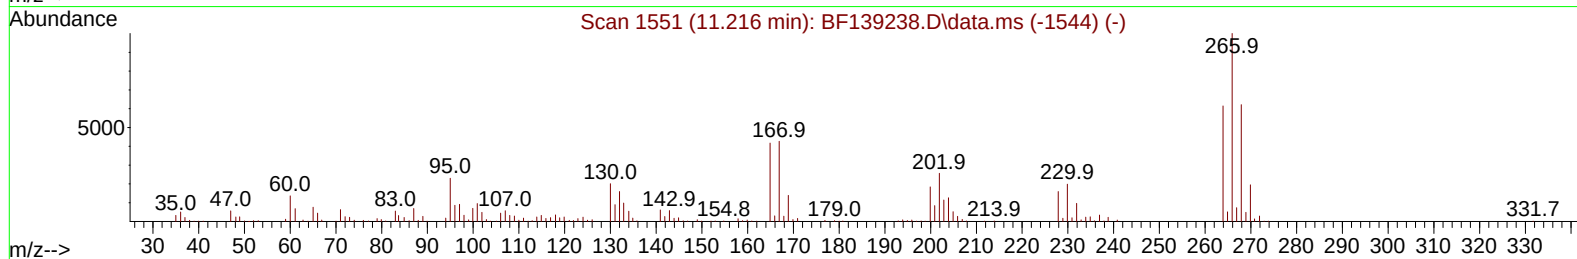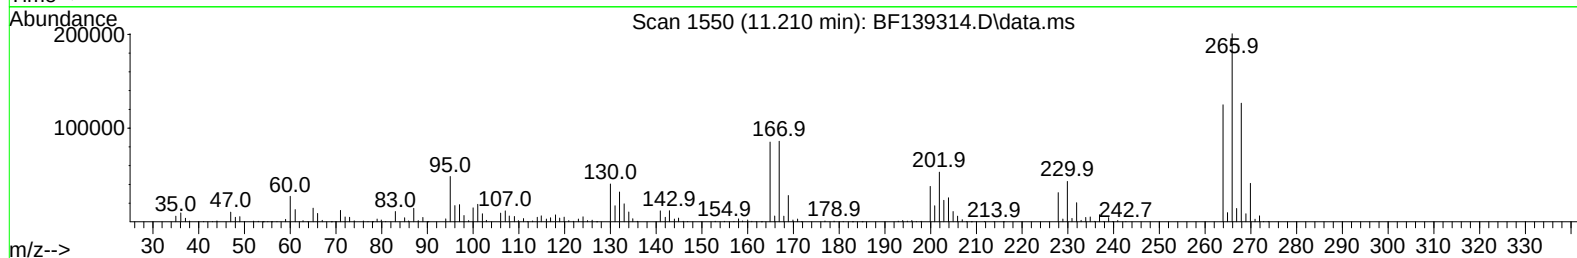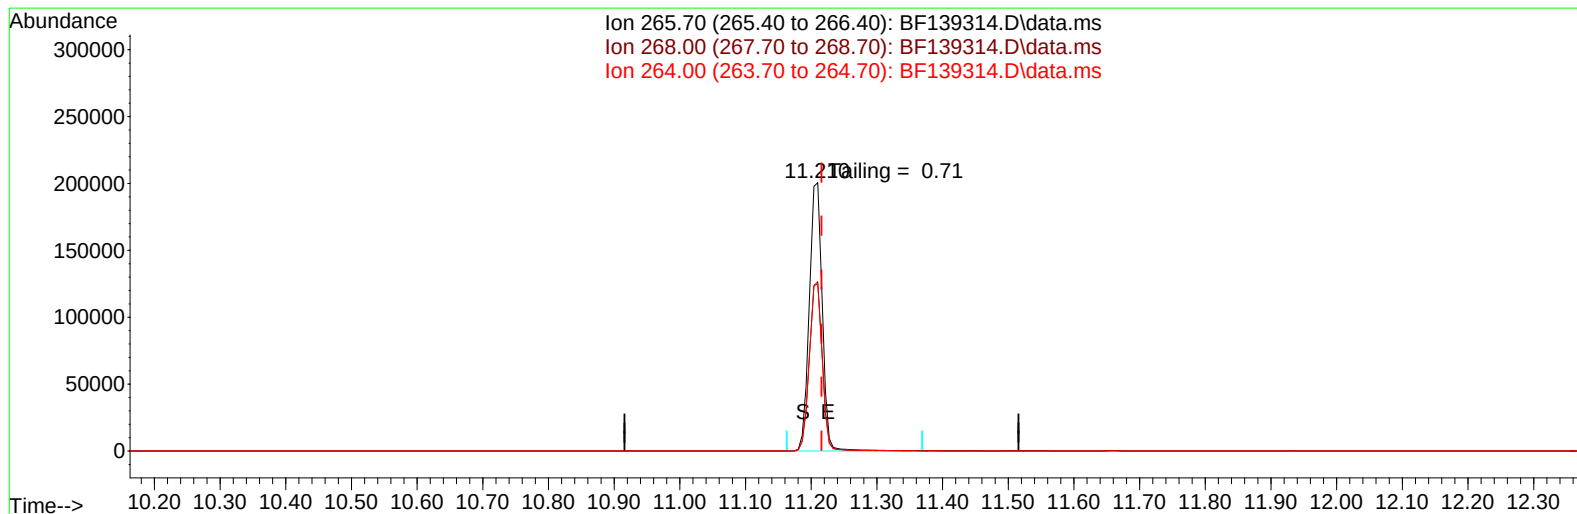

TIC: BF139314.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.006) 43719.77 ng




response 275456

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	63.08
264.00	61.50	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091124\
Data File : BF139314.D
Acq On : 11 Sep 2024 09:52
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 11 11:06:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

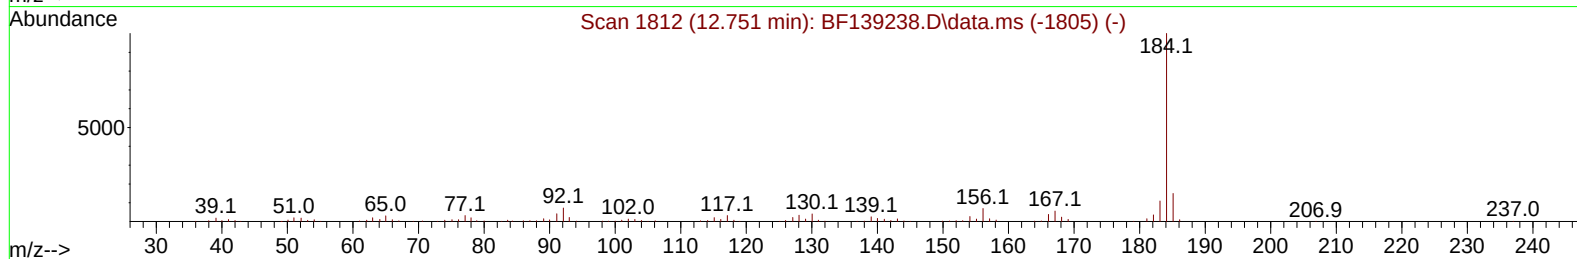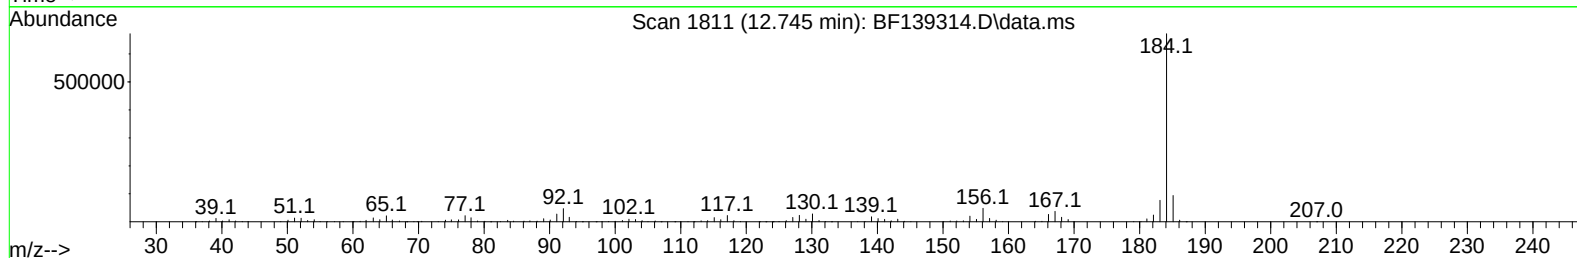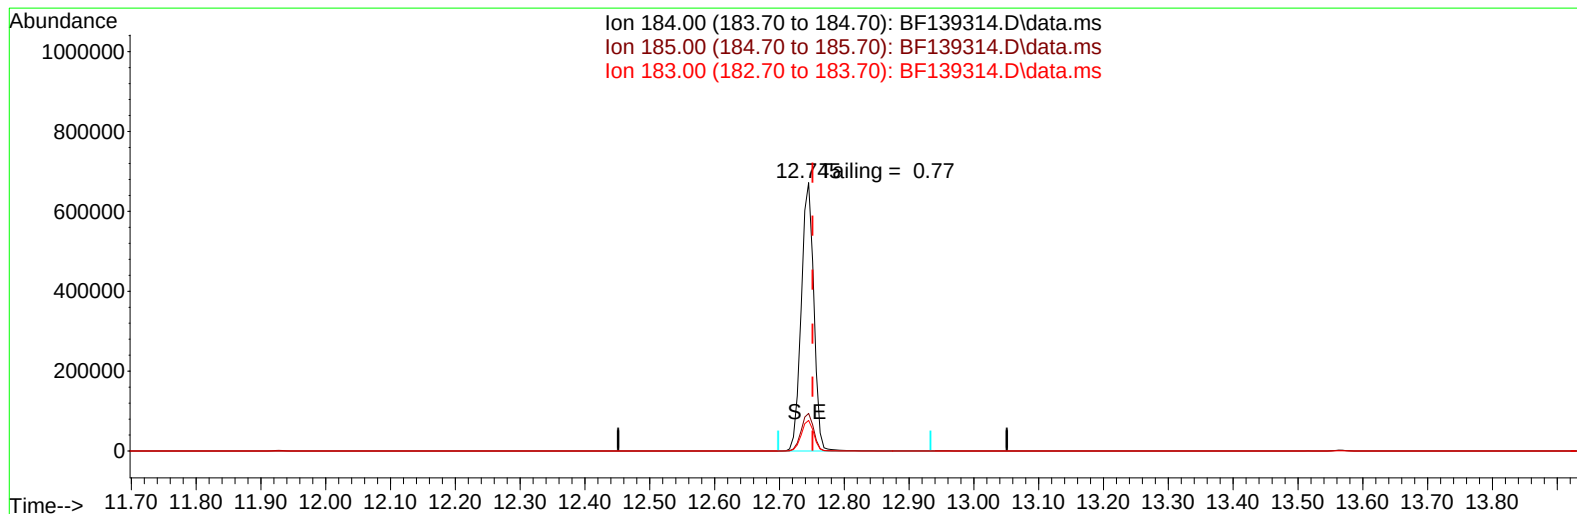

TIC: BF139314.D\data.ms

(77) Benzidine

12.745min (-0.006) 0.00 ng

response 906153

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.02
183.00	11.00	11.42
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/11/2024	BNA_F	<u>BF139314.D</u>
Compound Name	Response	Retention Time
DDT	581834	13.563
DDD	13574	13.263
DDE	757	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14331	596165	2.40

Instrument :
BNA_F
ClientSampleId :
DFTPP