


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF091216\
 Data File : BF090055.D
 Acq On : 12 Sep 2016 11:12
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF083116.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 08 16:07:52 2016

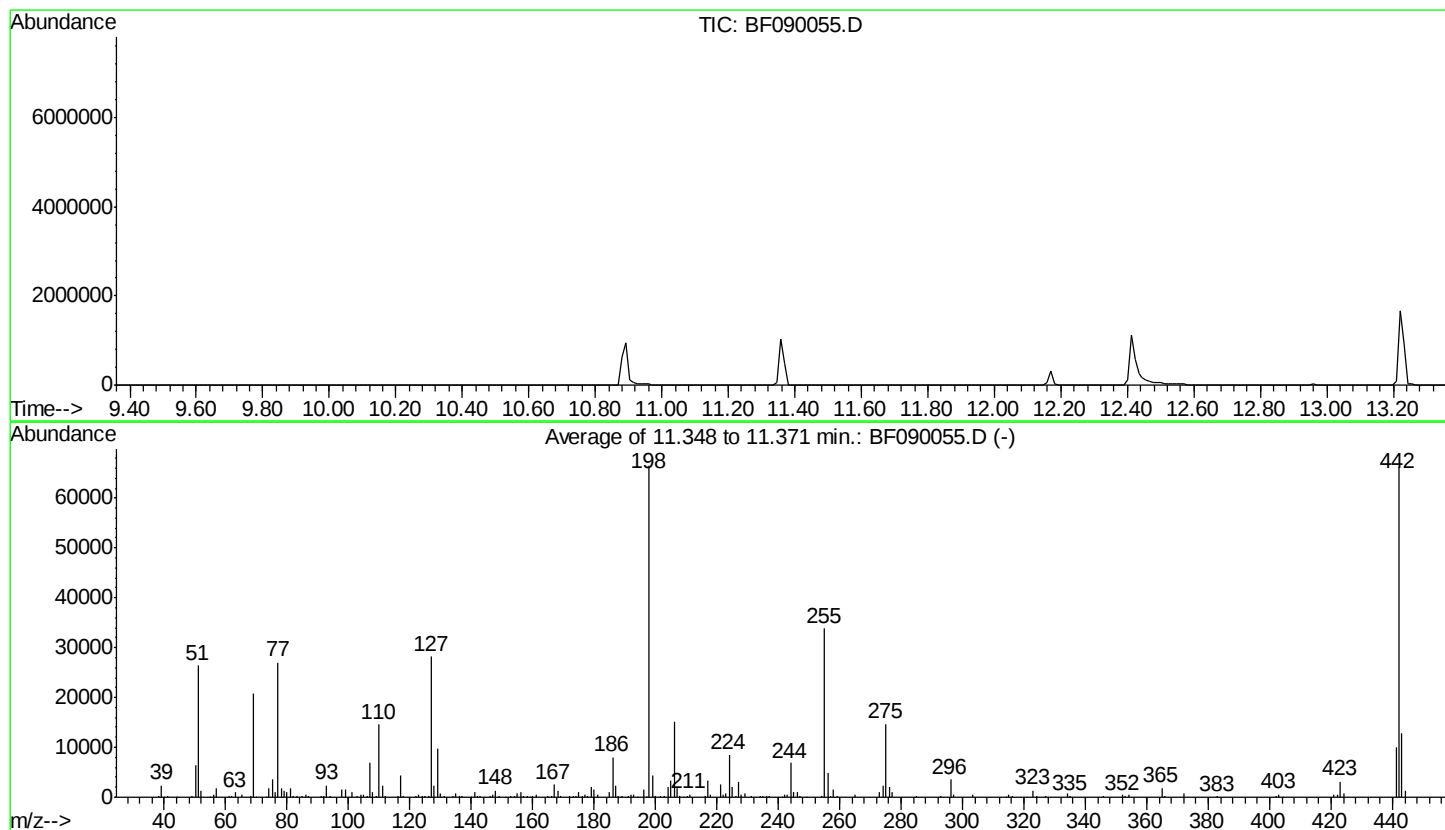

AutoFind: Scans 854, 855, 856; Background Corrected with Scan 851

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	26381	PASS
68	69	0.00	2	1.2	253	PASS
69	198	0.00	100	31.2	20751	PASS
70	69	0.00	2	0.5	103	PASS
127	198	10	80	42.4	28172	PASS
197	198	0.00	2	0.2	116	PASS
198	198	100	100	100.0	66502	PASS
199	198	5	9	6.5	4347	PASS
275	198	10	60	22.1	14669	PASS
365	198	1	100	2.8	1872	PASS
441	442	0.01	24	15.0	9946	PASS
442	198	50	100	99.6	66221	PASS
443	442	15	24	19.5	12910	PASS