
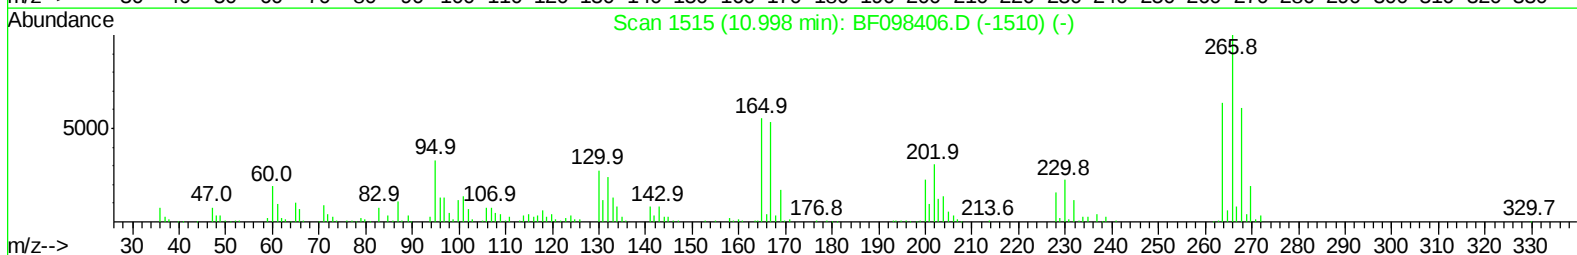
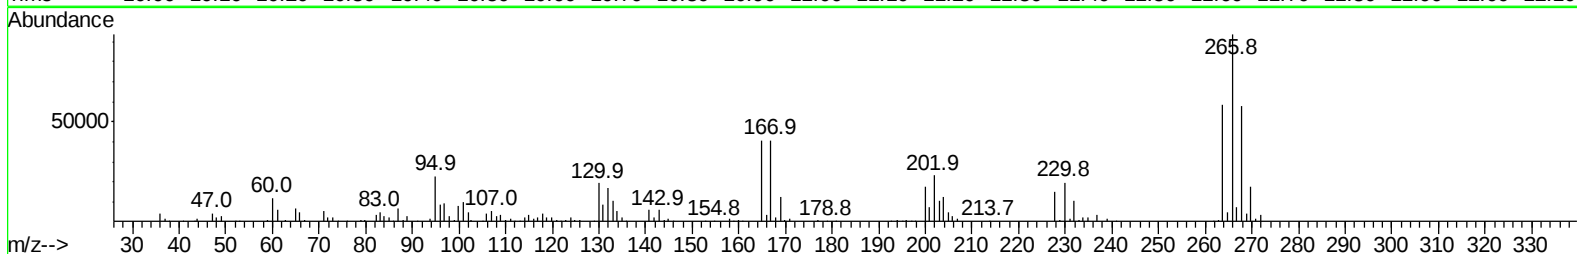


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF091217\
Data File : BF098446.D
Acq On : 12 Sep 2017 13:18
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 17:55:11 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

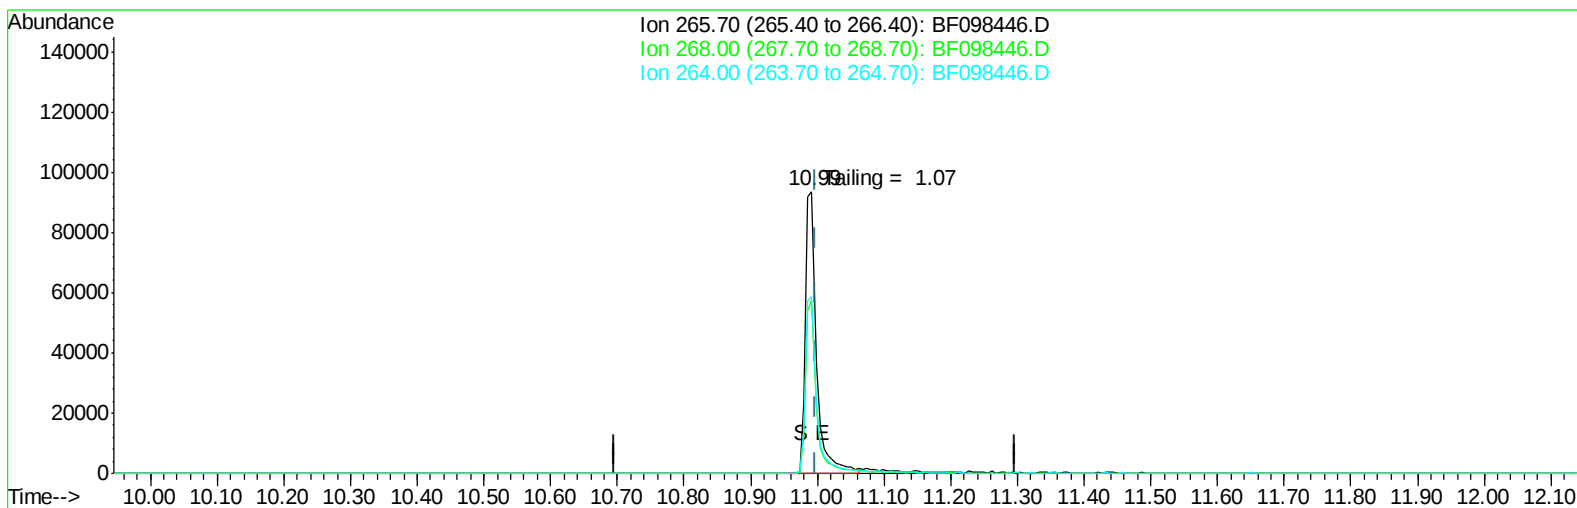

TIC: BF098446.D

(69) Pentachlorophenol (C)




10.992min (-0.005) 37704.77ng

response 108886

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.57
264.00	64.60	62.81
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF091217\
 Data File : BF098446.D
 Acq On : 12 Sep 2017 13:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 17:55:11 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 02:14:50 2017
 Response via : Initial Calibration

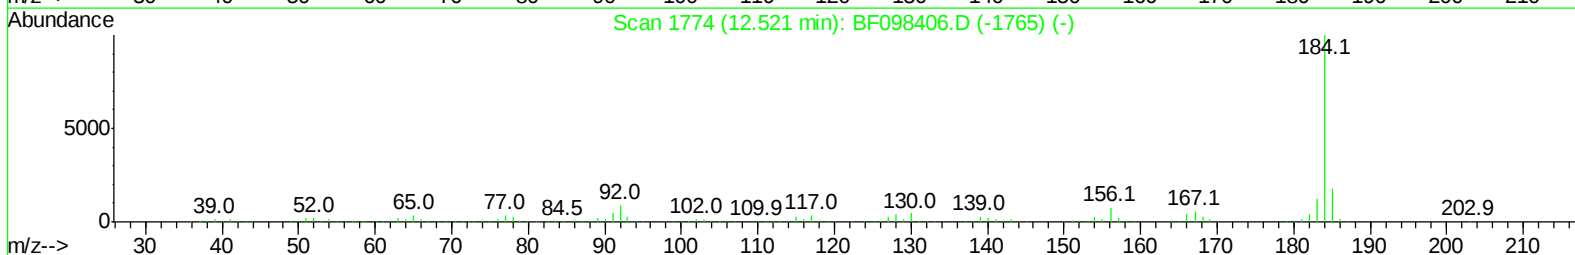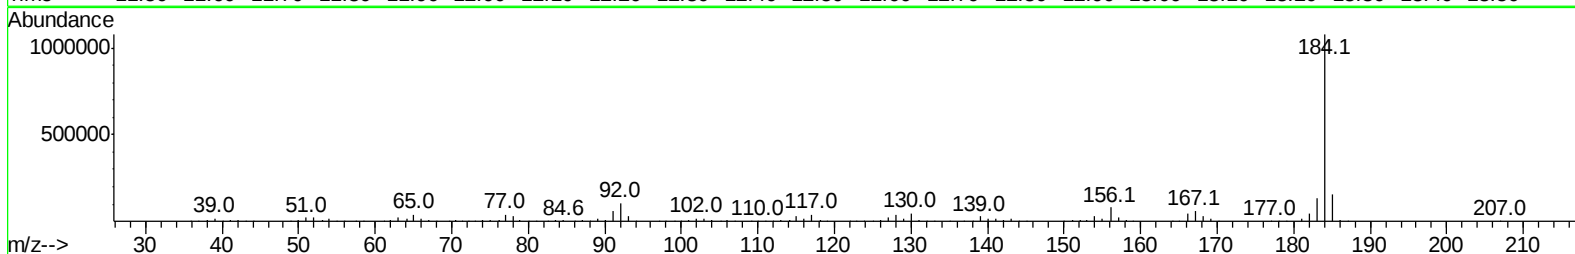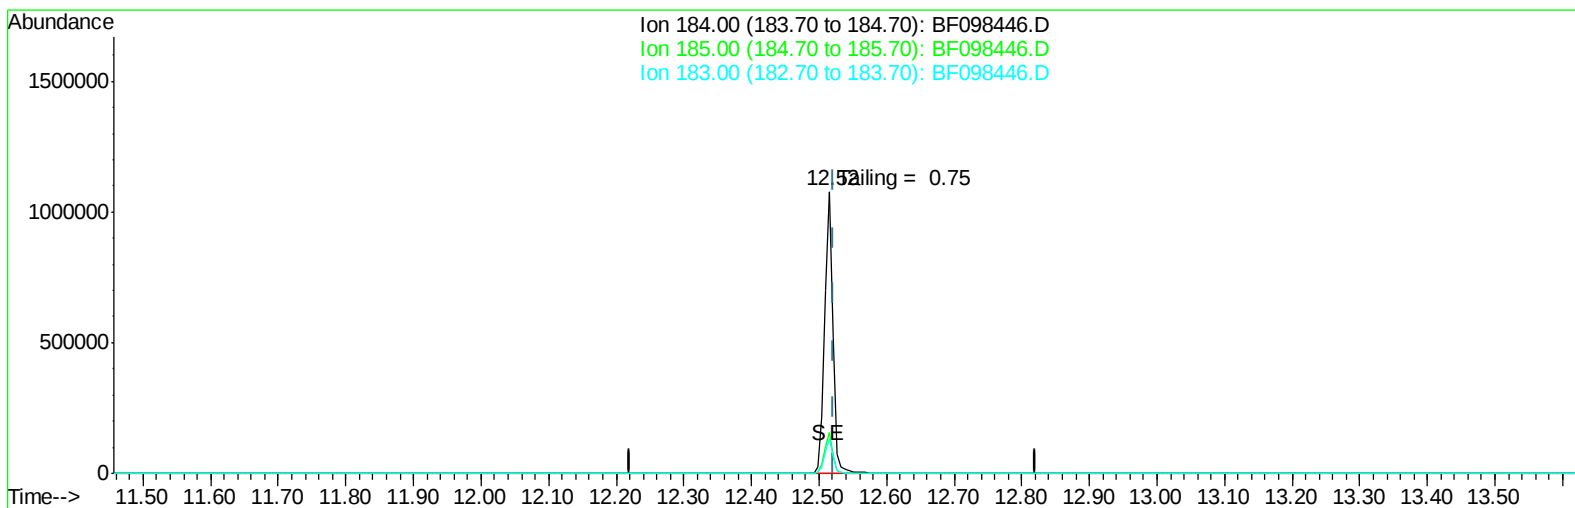

TIC: BF098446.D

(76) Benzidine

12.515min (-0.006) 0.00ng

response 949629

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.56#
183.00	12.20	12.42
0.00	0.00	0.00