
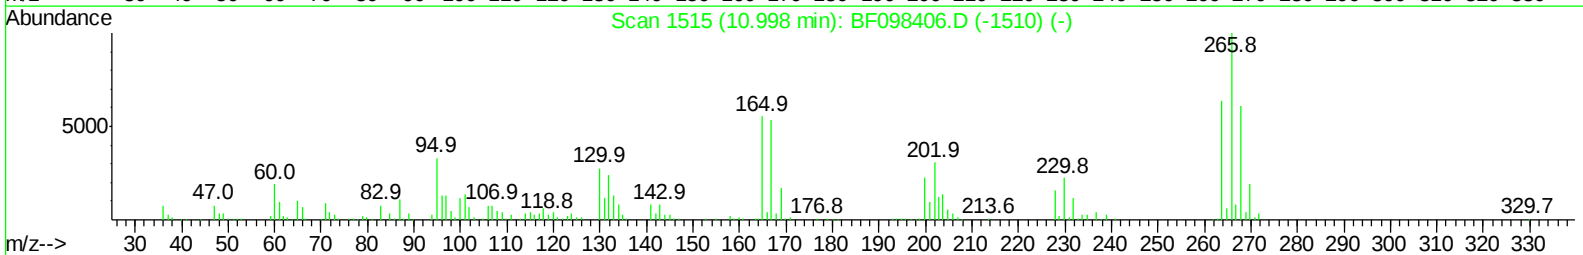
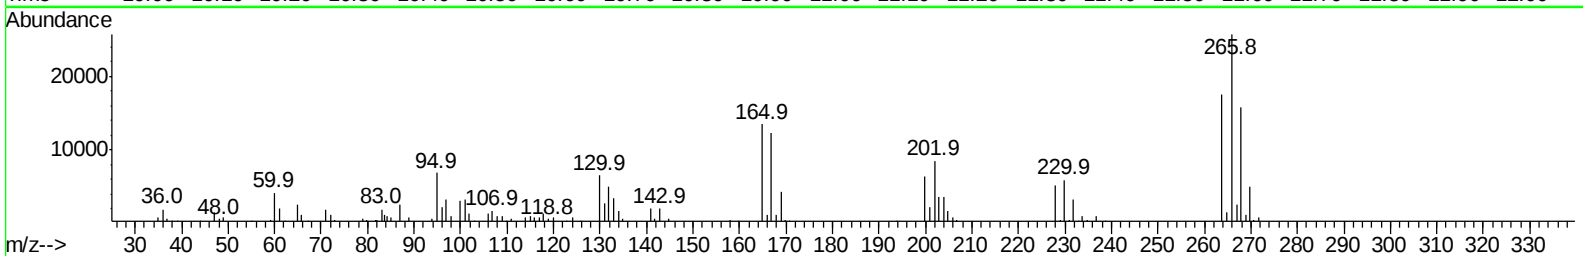


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF091217\
Data File : BF098472.D
Acq On : 13 Sep 2017 1:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 18:12:24 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

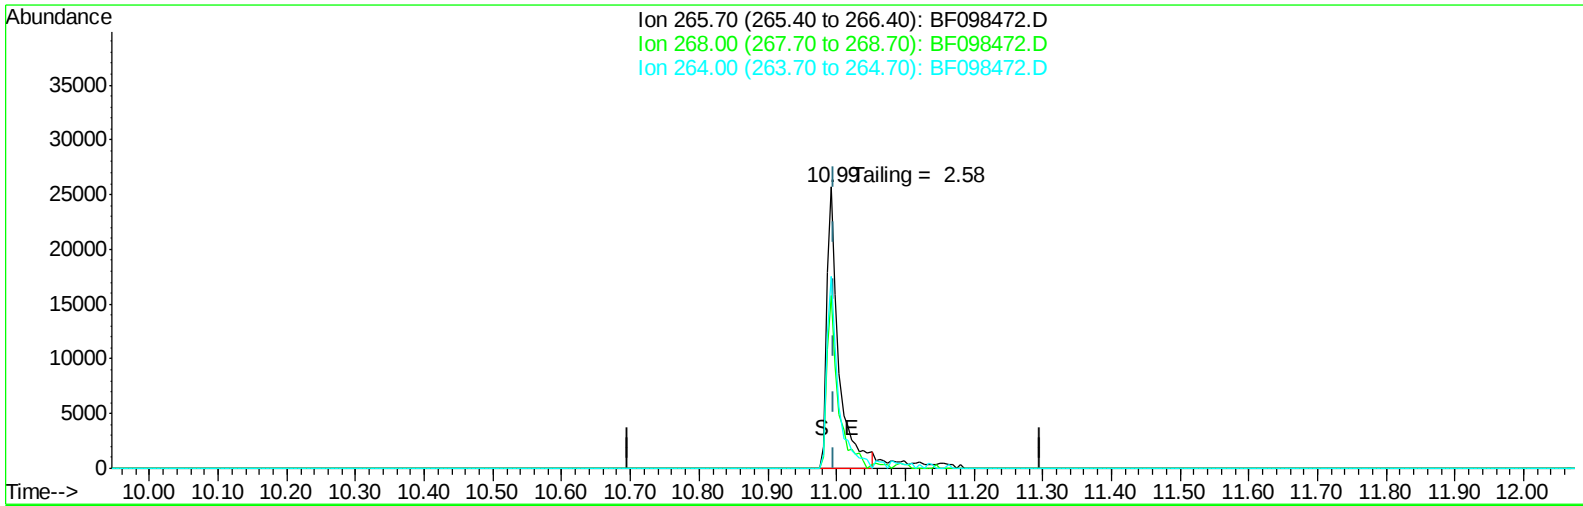

TIC: BF098472.D

(69) Pentachlorophenol (C)




10.992min (-0.005) 16673.22ng

response 32585

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	61.32
264.00	64.60	68.42
0.00	0.00	0.00

Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF091217\
Data File : BF098472.D
Acq On : 13 Sep 2017 1:53
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 18:12:24 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

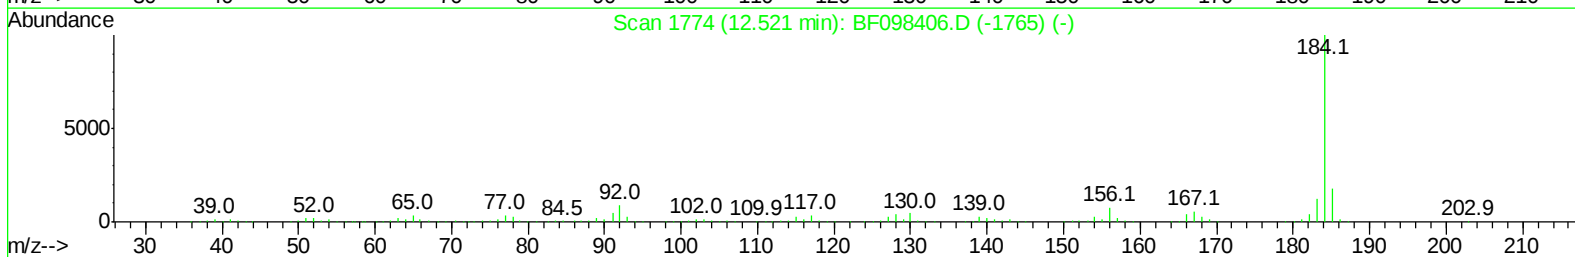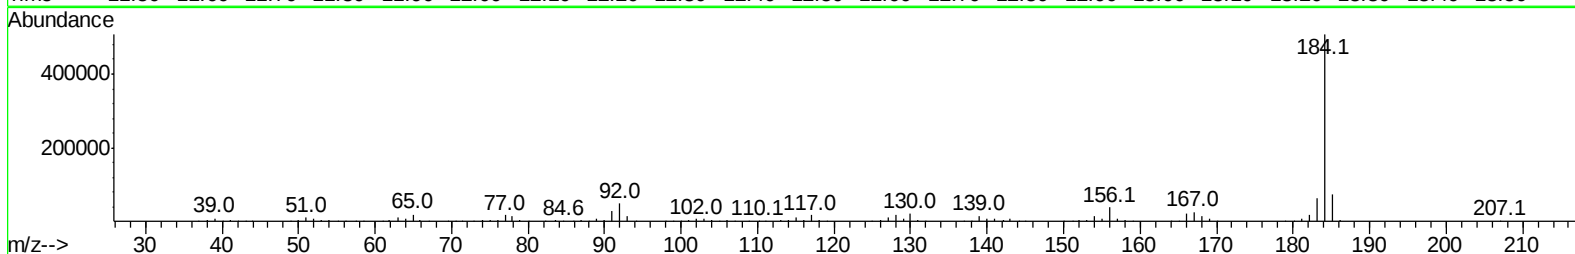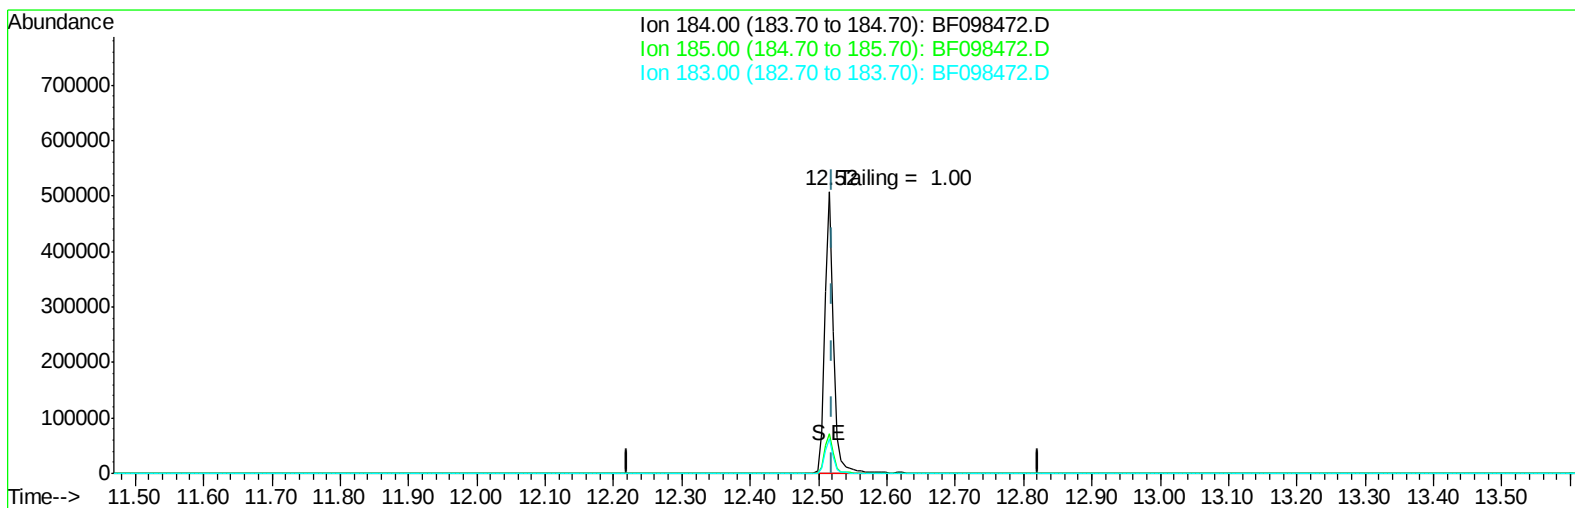

TIC: BF098472.D

(76) Benzidine

12.516min (-0.006) 0.00ng

response 461601

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.29#
183.00	12.20	12.29
0.00	0.00	0.00