

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF091217\
 Data File : BF098480.D
 Acq On : 13 Sep 2017 5:36
 Operator : SJ/JU
 Sample : I5181-01
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 090817-TIDO-F-D-M

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.263	536	540	557	rBV	3808409	3885184	79.11%	10.908%
2	6.310	714	718	735	rBV	3726947	3696927	75.27%	10.380%
3	6.434	735	739	742	rBV	4226940	3723426	75.81%	10.454%
4	6.663	774	778	787	rVB	1269397	1119788	22.80%	3.144%
5	6.816	800	804	808	rBV	3900211	3841118	78.21%	10.784%
6	7.234	870	875	878	rBV	3343923	3065616	62.42%	8.607%
7	7.945	992	996	1010	rBV	1682715	1413506	28.78%	3.969%
8	9.022	1173	1179	1182	rBV	5345569	4911325	100.00%	13.789%
9	9.692	1289	1293	1302	rVB	1405275	1304655	26.56%	3.663%
10	10.480	1424	1427	1440	rBV	1546279	1542277	31.40%	4.330%
11	11.174	1541	1545	1553	rBV	1380966	1154838	23.51%	3.242%
12	12.763	1810	1815	1818	rBV	4135220	3912098	79.65%	10.984%
13	13.810	1988	1993	1998	rBV	1131718	1077653	21.94%	3.026%
14	14.639	2132	2134	2137	rVB	69464	65220	1.33%	0.183%
15	15.210	2227	2231	2237	rVB	654332	844935	17.20%	2.372%
16	15.621	2298	2301	2305	rBV3	39006	58940	1.20%	0.165%




Sum of corrected areas: 35617506

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF091217\
Data File : BF098480.D
Acq On : 13 Sep 2017 5:36
Operator : SJ/JU
Sample : I5181-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
090817-TIDO-F-D-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

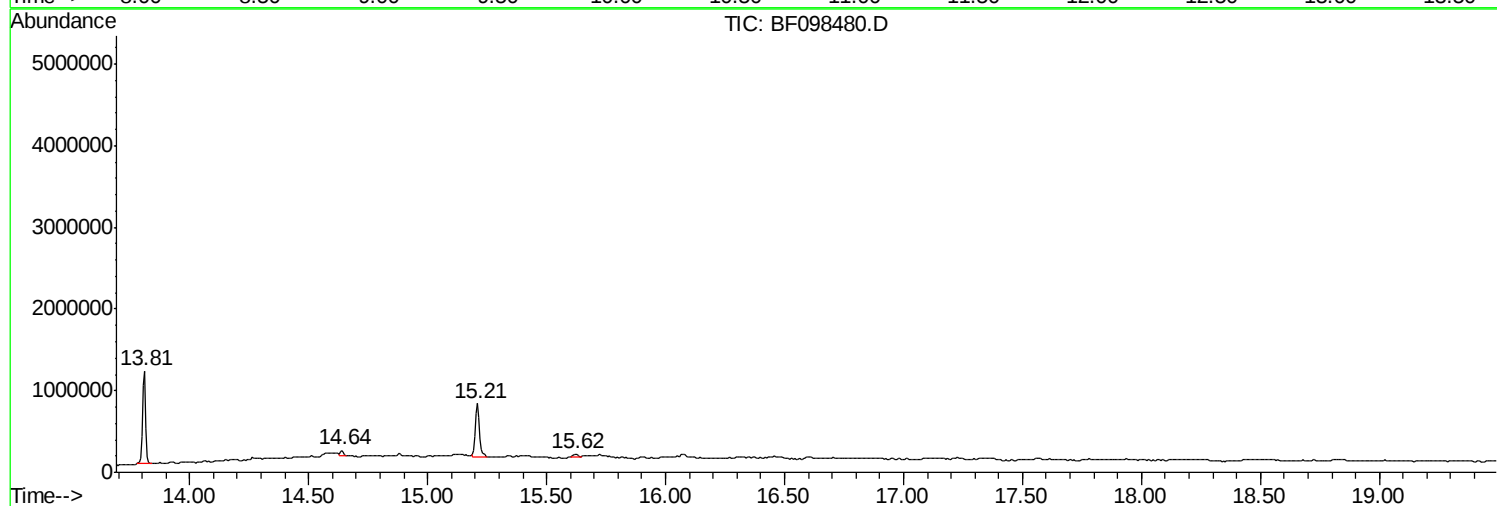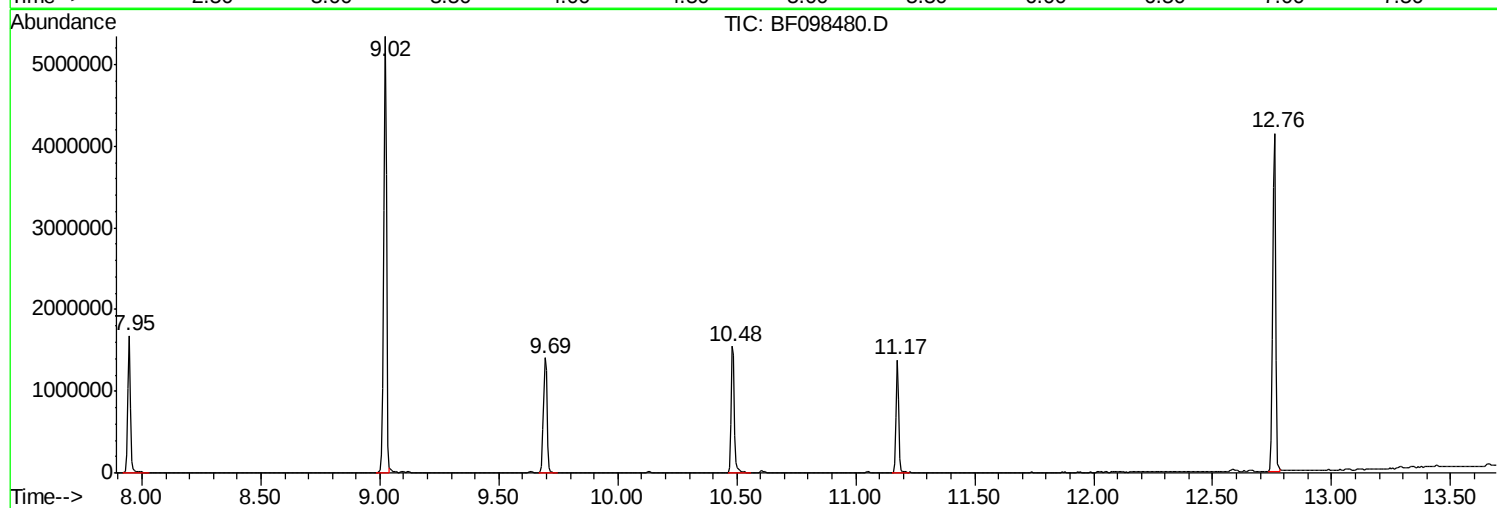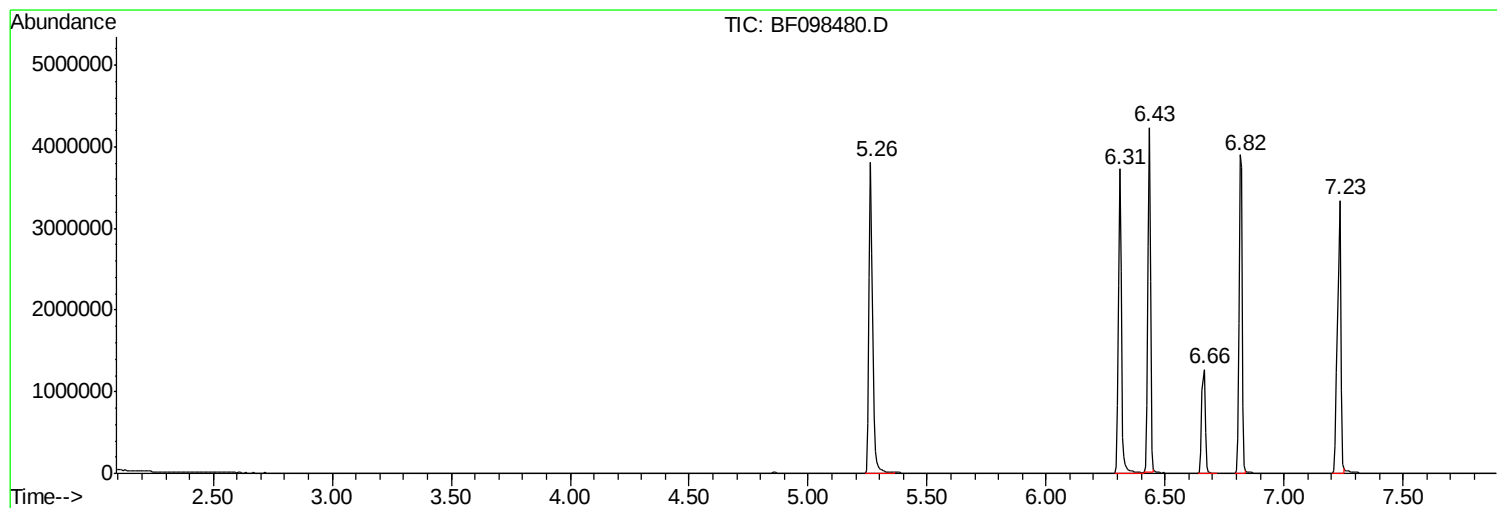

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF091217\
Data File : BF098480.D
Acq On : 13 Sep 2017 5:36
Operator : SJ/JU
Sample : I5181-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
090817-TIDO-F-D-M










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.43 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.43	66.50 ng	3723430	1,4-Dichlorobenzene-d4	6.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9

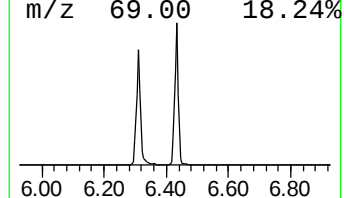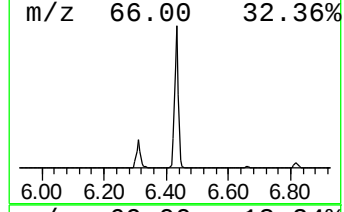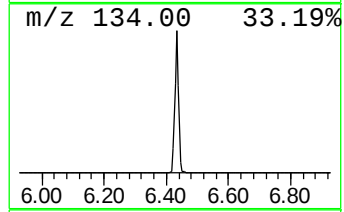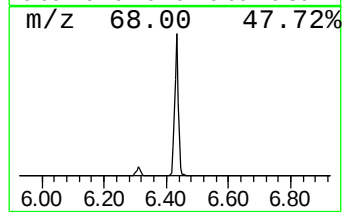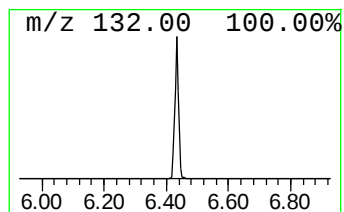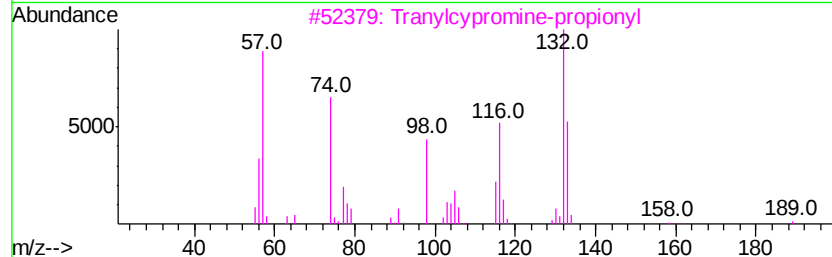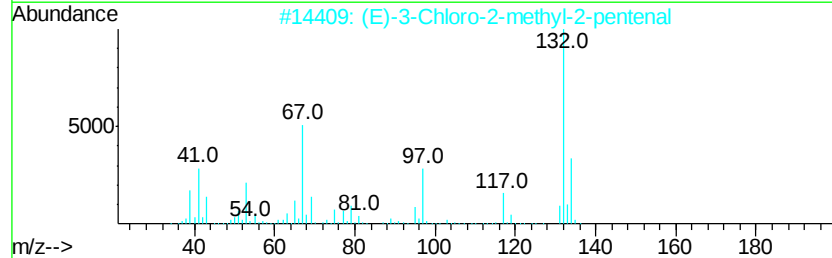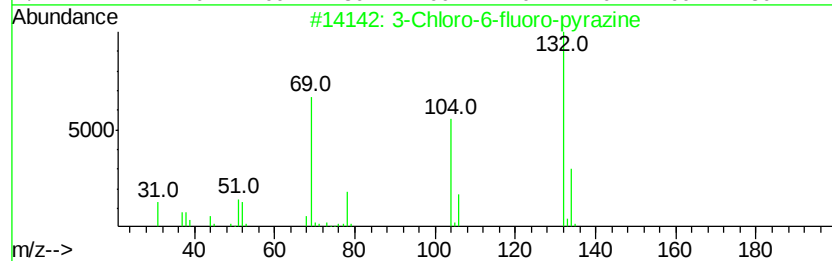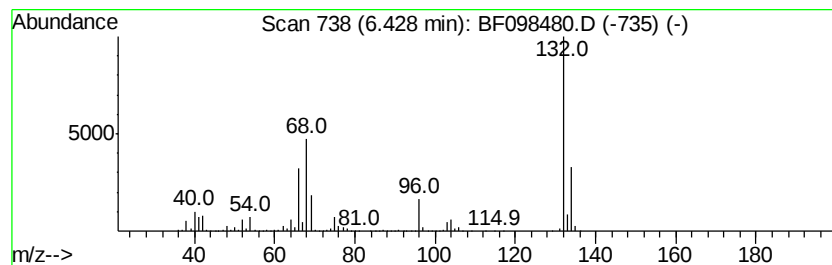

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF091217\
Data File : BF098480.D
Acq On : 13 Sep 2017 5:36
Operator : SJ/JU
Sample : I5181-01
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
090817-TIDO-F-D-M

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.43	6.43	66.5	ng	3723430	1	6.66	1119790	20.0