


Data Path : Z:\HPCHEM1\BNA F\Data\BF091217\
 Data File : BF098446.D
 Acq On : 12 Sep 2017 13:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Sep 12 02:14:50 2017

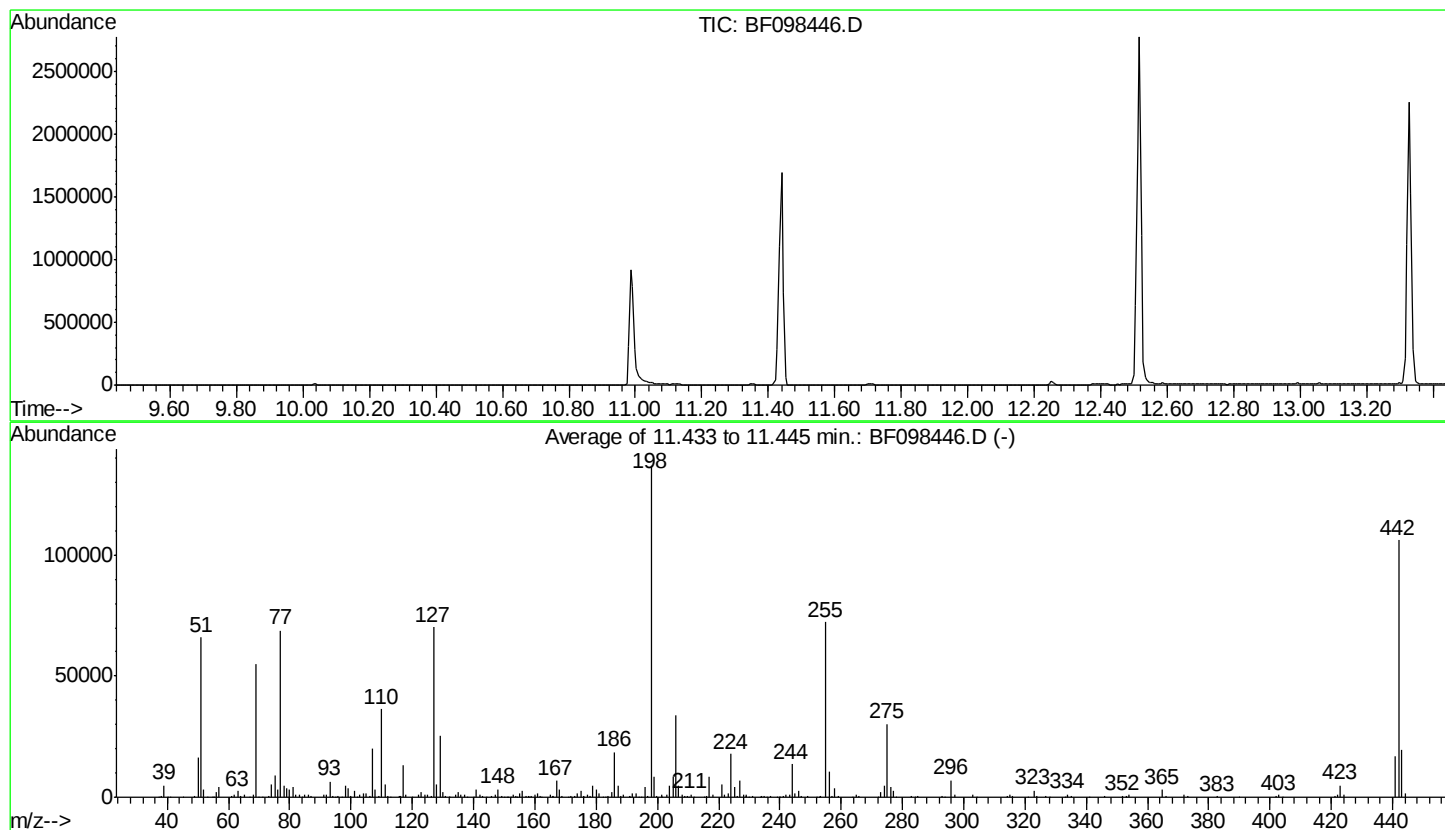

AutoFind: Scans 1589, 1590, 1591; Background Corrected with Scan 1583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.1	65850	PASS
68	69	0.00	2	2.0	1088	PASS
69	198	0.00	100	40.3	55173	PASS
70	69	0.00	2	0.5	280	PASS
127	198	10	80	51.3	70210	PASS
197	198	0.00	2	0.2	327	PASS
198	198	100	100	100.0	136877	PASS
199	198	5	9	6.2	8454	PASS
275	198	10	60	22.1	30285	PASS
365	198	1	100	2.3	3105	PASS
441	442	0.01	24	15.8	16791	PASS
442	198	50	100	77.5	106069	PASS
443	442	15	24	18.7	19830	PASS