
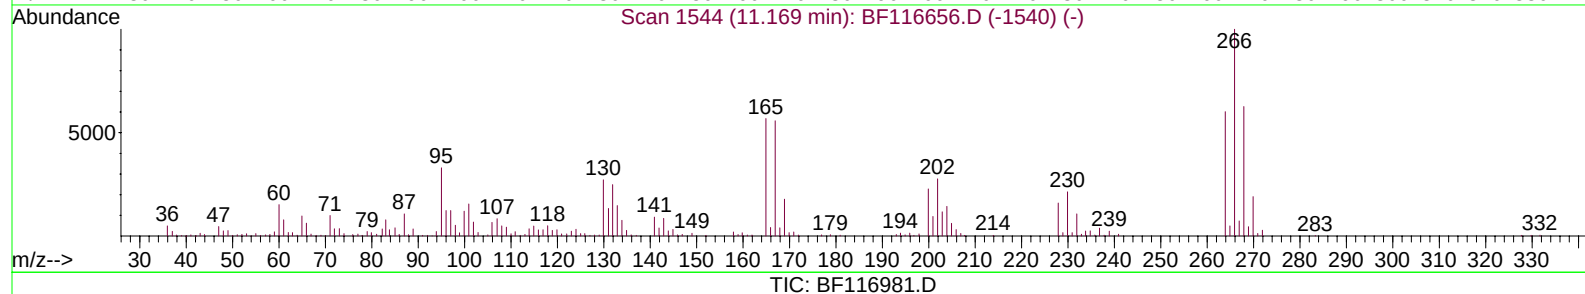
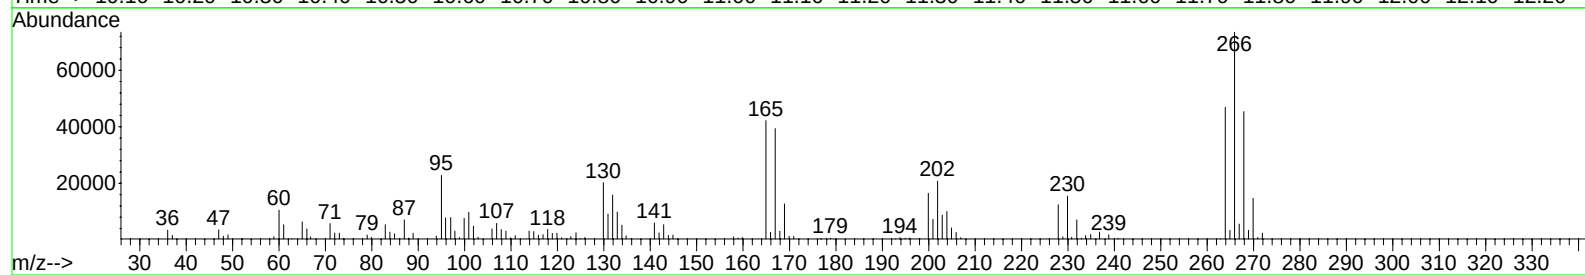


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091219\
Data File : BF116981.D
Acq On : 12 Sep 2019 9:45
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 18:19:52 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 12 08:24:39 2019
Response via : Initial Calibration

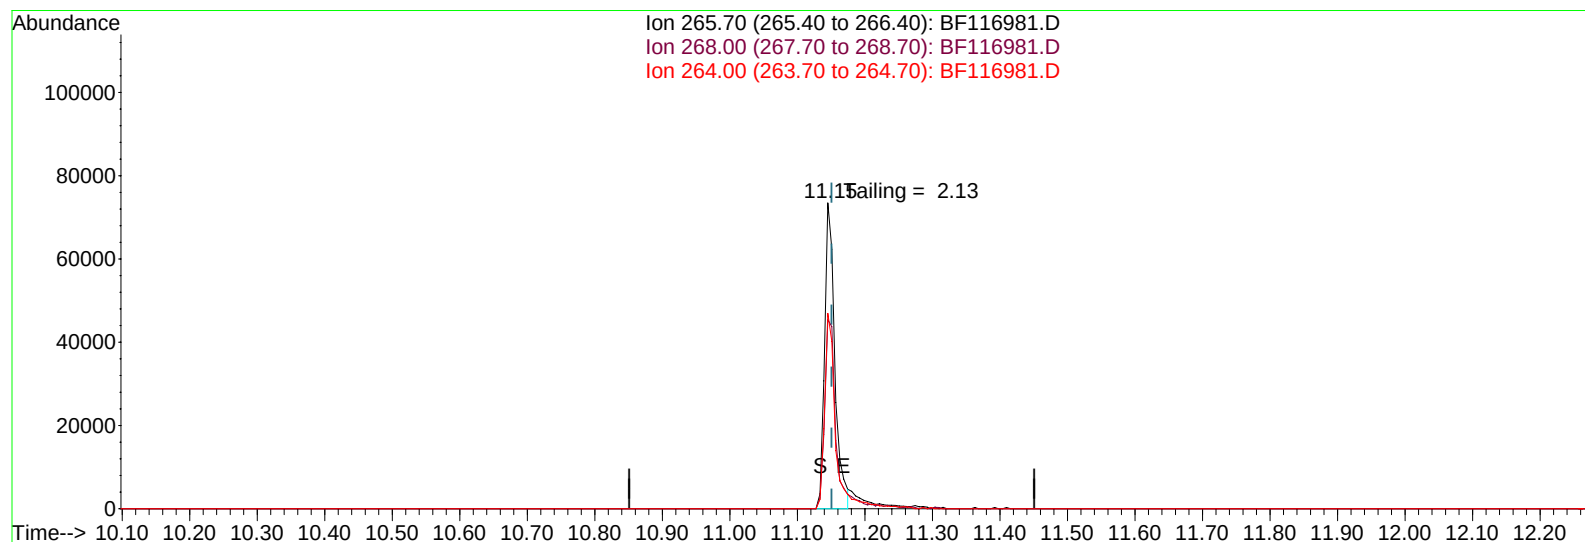

(70) Pentachlorophenol (C)




11.145min (-0.006) 40874.29ng

response 85534

Ion	Exp%	Act%
265.70	100	100
268.00	64.30	61.81
264.00	65.10	63.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF091219\
 Data File : BF116981.D
 Acq On : 12 Sep 2019 9:45
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 18:19:52 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 12 08:24:39 2019
 Response via : Initial Calibration

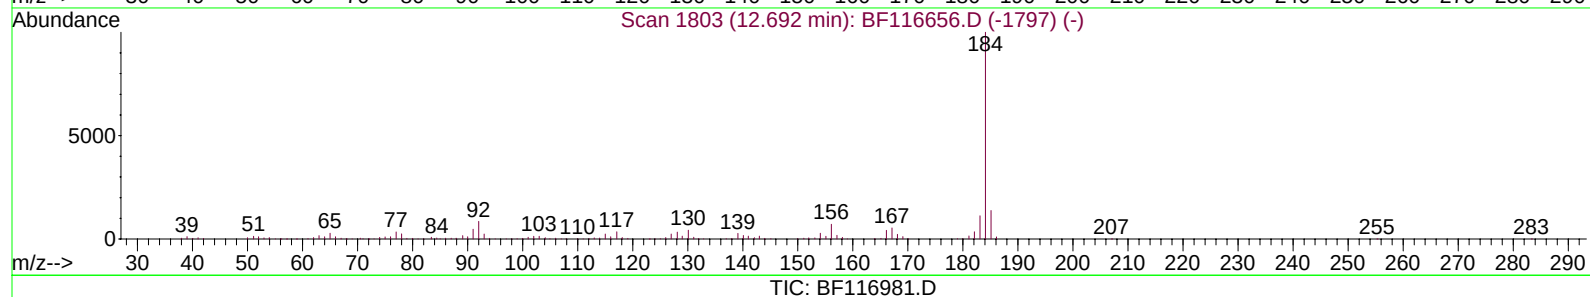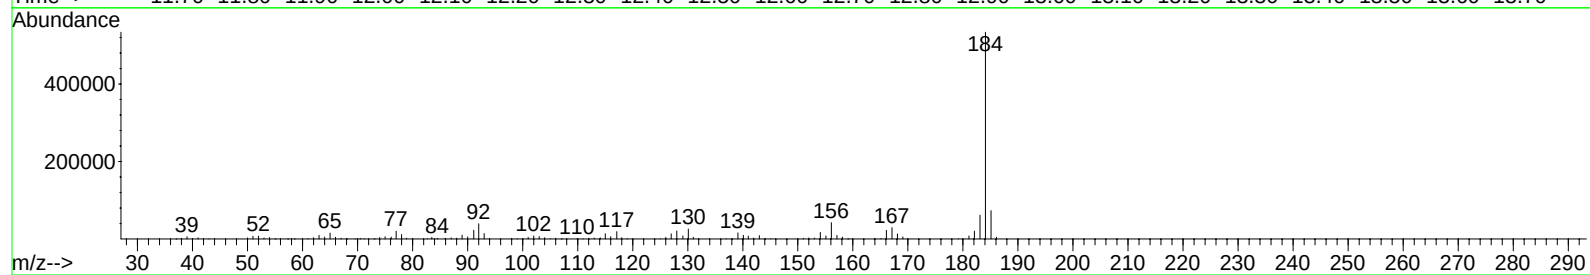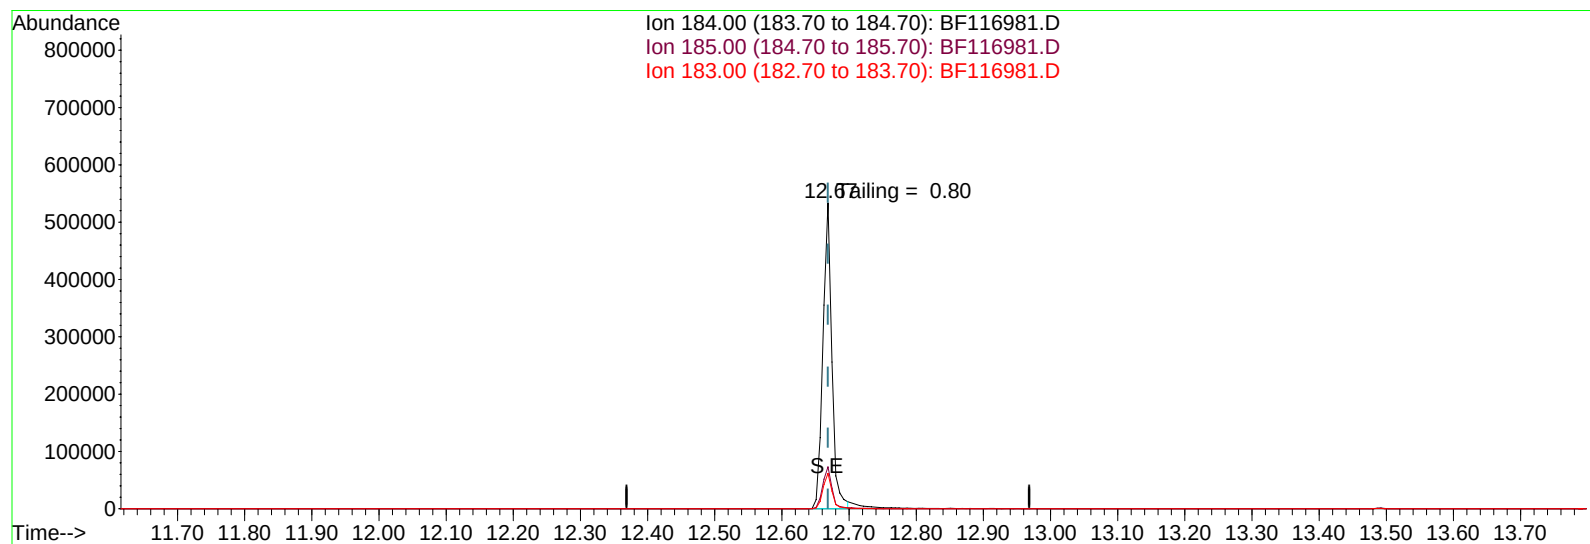

(77) Benzidine

12.669min (+0.000) 0.00ng

response 511847

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	13.73
183.00	11.50	11.59
0.00	0.00	0.00