

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091219\
 Data File : BF117002.D
 Acq On : 12 Sep 2019 19:50
 Operator : HP/JU
 Sample : K4850-04 2X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AOC-7-(8)

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:59:49 AM

Quant Time: Sep 13 08:27:32 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Sep 12 08:24:39 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.83	152	74862	20.00	ng	0.00
21) Naphthalene-d8	8.10	136	305903	20.00	ng	0.00
39) Acenaphthene-d10	9.86	164	167725	20.00	ng	0.00
64) Phenanthrene-d10	11.34	188	226947	20.00	ng	0.00
76) Chrysene-d12	13.98	240	167446	20.00	ng	0.00
87) Perylene-d12	15.44	264	164503	20.00	ng	0.02
System Monitoring Compounds						
5) 2-Fluorophenol	5.44	112	170038	36.80	ng	0.00
7) Phenol-d6	6.45	99	227720	37.53	ng	-0.01
23) Nitrobenzene-d5	7.38	82	137248	25.61	ng	-0.01
42) 2,4,6-Tribromophenol	10.64	330	43356	38.67	ng	0.00
45) 2-Fluorobiphenyl	9.17	172	193595	19.47	ng	0.00
79) Terphenyl-d14	12.92	244	140726	15.55	ng	0.00
Target Compounds						Qvalue
31) Naphthalene	8.13	128	580467	39.906	ng	98
37) 2-Methylnaphthalene	8.82	142	254974	26.345	ng	# 89
38) 1-Methylnaphthalene	8.92	142	178101	19.494	ng	# 99
46) 1,1'-Biphenyl	9.28	154	40836	3.209	ng	99
49) Acenaphthylene	9.72	152	231004	15.160	ng	98
50) Dimethylphthalate	9.57	163	39875	3.444	ng	# 50
52) Acenaphthene	9.89	154	19760	2.111	ng	# 86
55) Dibenzofuran	10.06	168	30686	2.325	ng	# 87
58) Fluorene	10.40	166	133714	13.296	ng	97
71) Phenanthrene	11.37	178	729352	57.732	ng	99
72) Anthracene	11.42	178	103475	8.137	ng	99
75) Fluoranthene	12.56	202	397886	32.048	ng	97
78) Pyrene	12.79	202	647179	43.479	ng	100
81) Benzo(a)anthracene	13.97	228	290280	27.391	ng	98
83) Chrysene	14.01	228	316904	29.025	ng	98
86) Indeno(1,2,3-cd)pyrene	16.87	276	85063	9.700	ng	95
88) Benzo(b)fluoranthene	15.02	252	253556m	25.494	ng	
89) Benzo(k)fluoranthene	15.03	252	97760m	10.781	ng	
90) Benzo(a)pyrene	15.37	252	155549	17.977	ng	99
91) Dibenzo(a,h)anthracene	16.87	278	28309m	3.738	ng	
92) Benzo(g,h,i)perylene	17.30	276	79011	10.229	ng	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091219\
Data File : BF117002.D
Acq On : 12 Sep 2019 19:50
Operator : HP/JU
Sample : K4850-04 2X
Misc :
ALS Vial : 22 Sample Multiplier: 1


Instrument :
BNA_F
ClientSampleId :
AOC-7-(8)

Manual Integrations
APPROVED

mohammad
9/16/2019 8:59:49 AM

Quant Time: Sep 13 08:27:32 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 12 08:24:39 2019
Response via : Initial Calibration

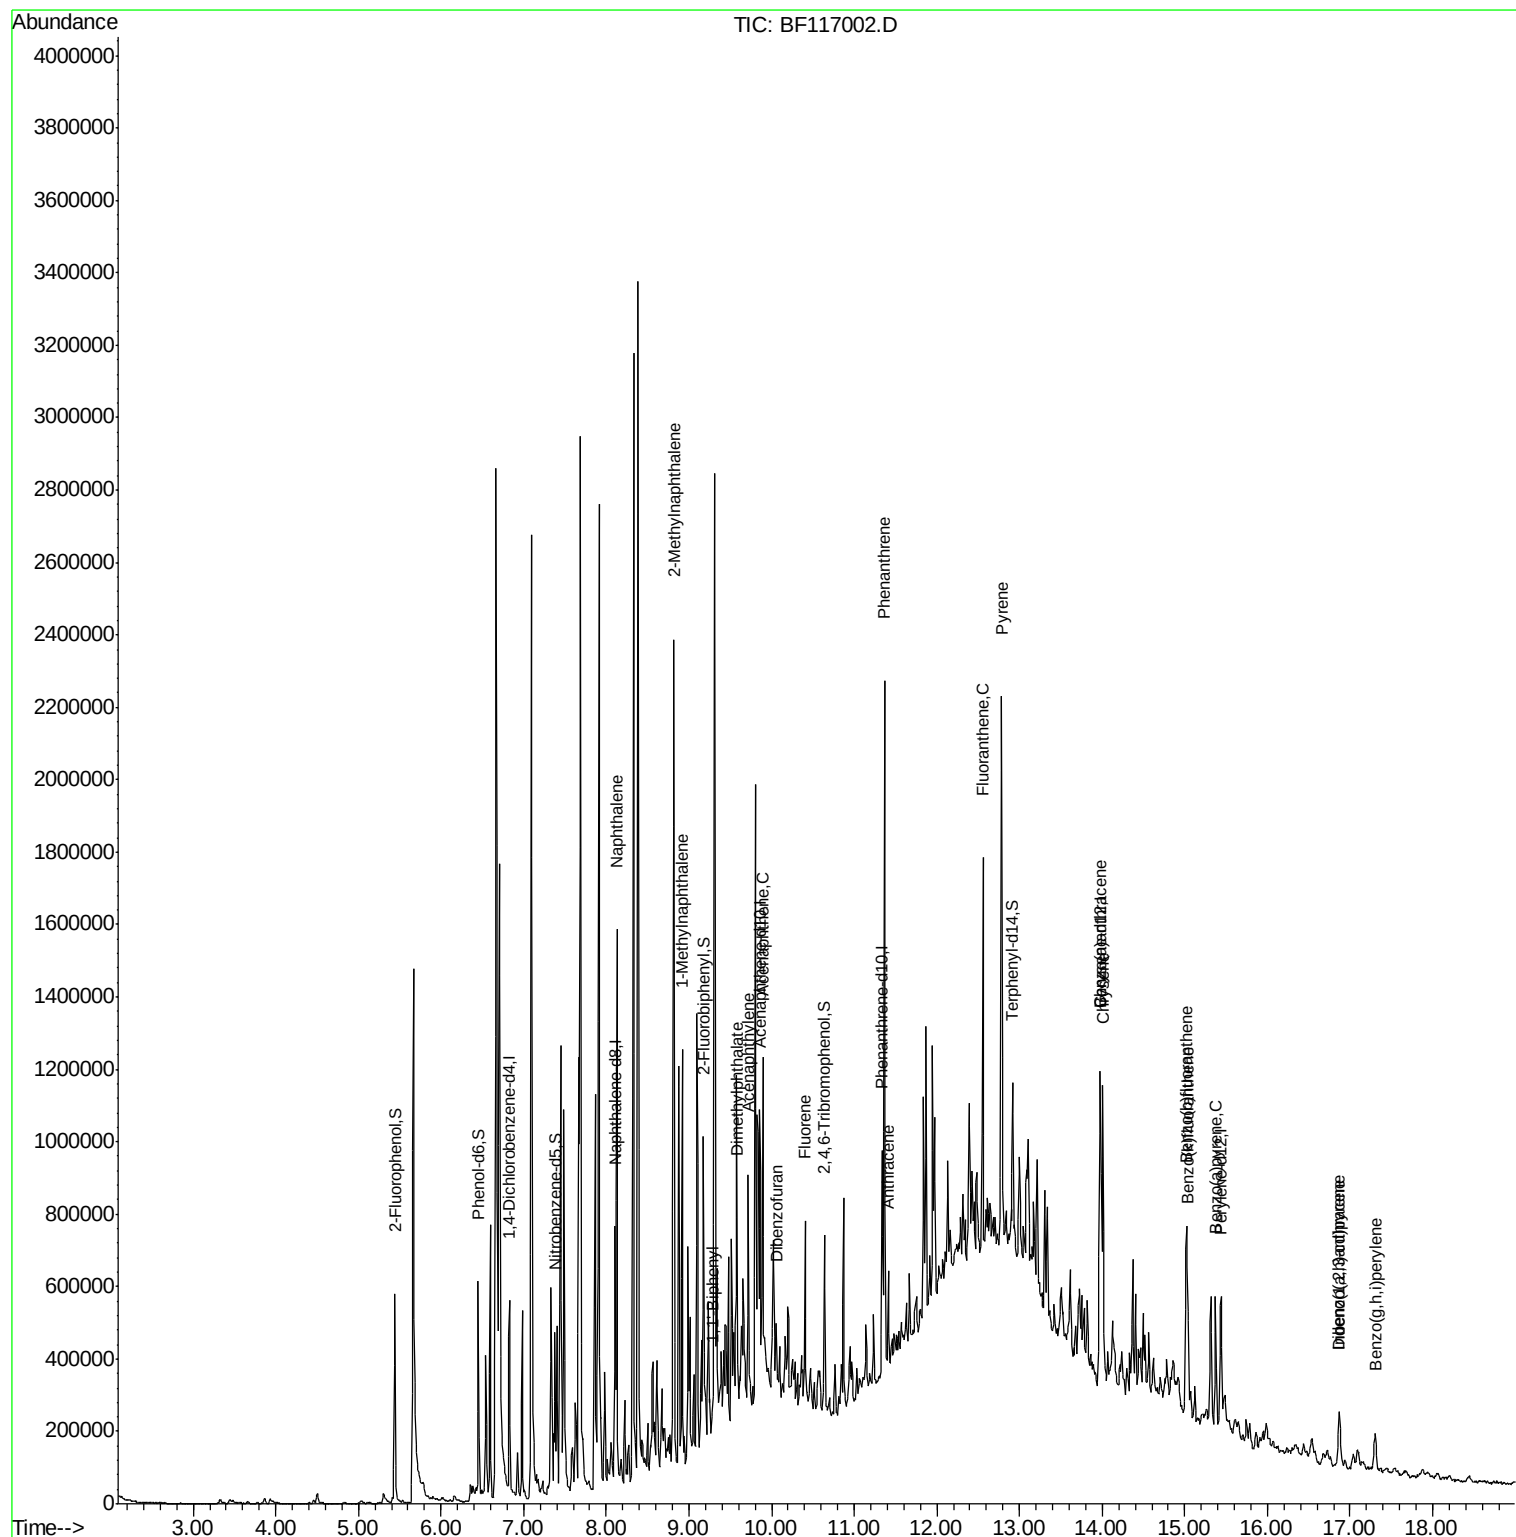

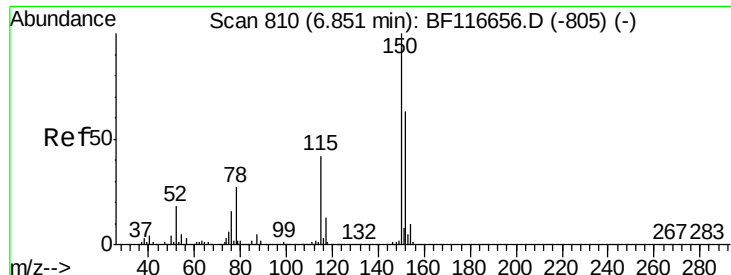

#1





1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.83 min Scan# 806
Delta R.T. -0.00 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Instrument :
BNA_F
ClientSampleId :
AOC-7-(8)

Tot Ion	Ratio	Lower	Upper
152	100		
150	154.5	126.2	189.2
115	66.6	50.2	75.2

Manual Integrations
APPROVED




mohammad
9/16/2019 8:59:49 AM

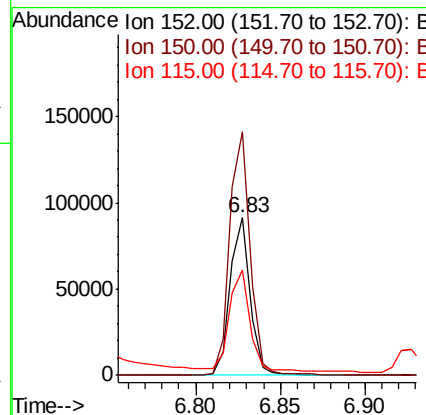


#5

2-Fluorophenol
Concen: 36.797 ng
RT: 5.44 min Scan# 570
Delta R.T. -0.00 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Tgt Ion	Ratio	Lower	Upper
112	100		
64	55.6	47.1	70.7
63	30.4	25.4	38.0

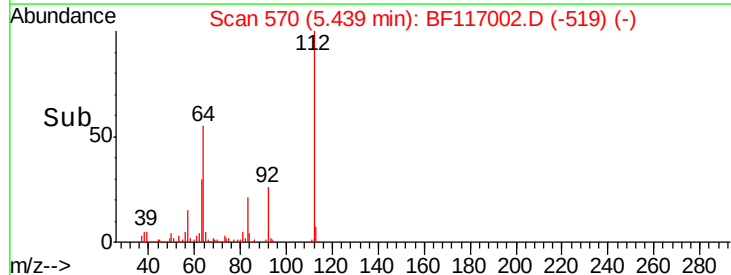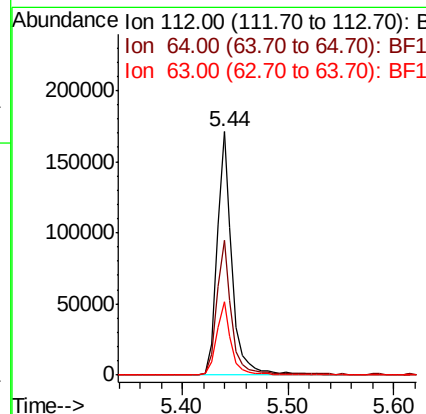



#7

Phenol-d6

Concen: 37.529 ng

RT: 6.45 min Scan# 742

Delta R.T. -0.01 min

Lab File: BF117002.D

Acq: 12 Sep 2019 19:50

Instrument :

BNA_F





ClientSampleId :

AOC-7-(8)

Tot Ion:	99	Resp:	227720
Ion Ratio	Lower	Upper	
99	100		
42	15.3	12.0	18.0
71	37.7	29.7	44.5

Manual Integrations
APPROVED

mohammad
9/16/2019 8:59:49 AM

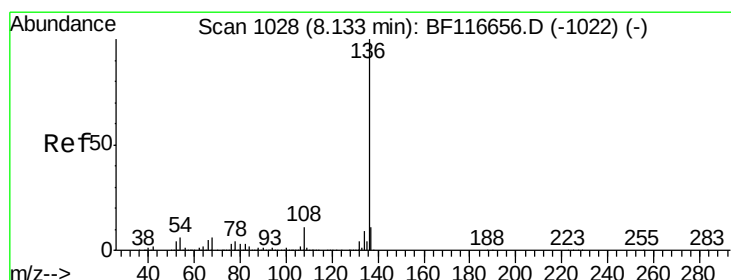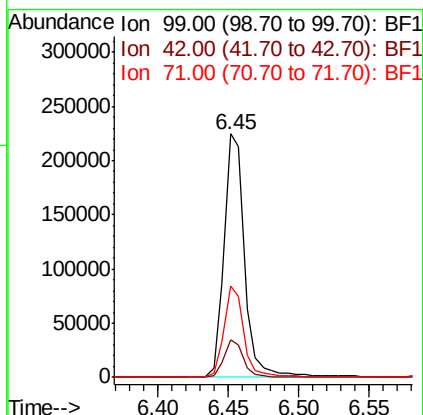

#21

Naphthalene-d8

Concen: 20.000 ng




RT: 8.10 min Scan# 1023


Delta R.T. -0.01 min

Lab File: BF117002.D

Acq: 12 Sep 2019 19:50

Tgt Ion:	136	Resp:	305903
Ion Ratio	Lower	Upper	
136	100		
137	10.4	8.5	12.7
54	5.6	3.8	5.8
68	5.4	3.6	5.4#

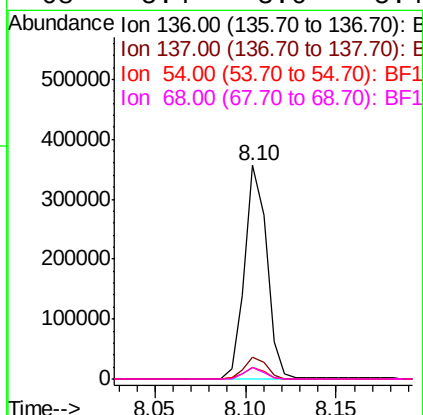



#23

Nitrobenzene-d5

Concen: 25.613 ng

RT: 7.38 min Scan# 900

Delta R.T. -0.01 min

Lab File: BF117002.D

Acq: 12 Sep 2019 19:50

Instrument :

BNA_F





ClientSampleId :

AOC-7(8)

Tot Ion	82	Resp	137248
Ion Ratio	Lower	Upper	
82	100		
128	41.3	35.0	52.4
54	38.2	32.6	48.8

Manual Integrations
APPROVED

mohammad
9/16/2019 8:59:49 AM

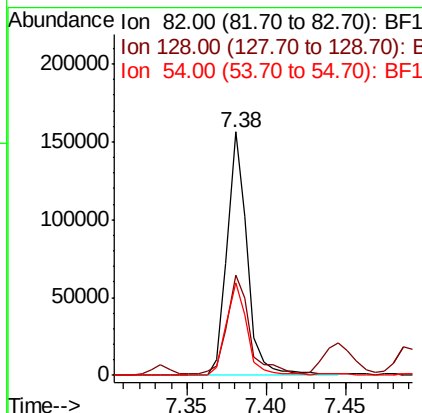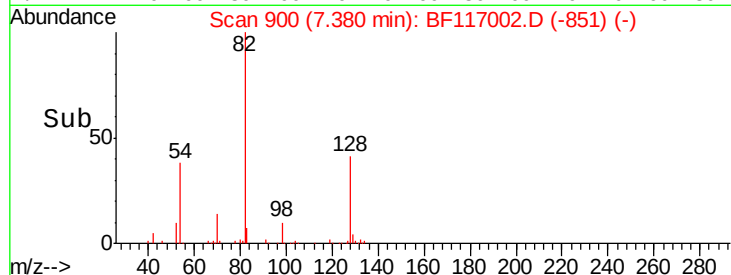

#31

Naphthalene

Concen: 39.906 ng




RT: 8.13 min Scan# 1027


Delta R.T. -0.00 min

Lab File: BF117002.D

Acq: 12 Sep 2019 19:50

Tgt Ion	128	Resp	580467
Ion Ratio	Lower	Upper	
128	100		
129	12.8	9.2	13.8
127	13.1	10.6	16.0

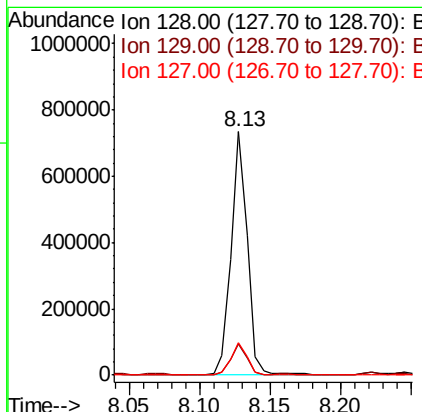







#37
2-Methylnaphthalene
Concen: 26.345 ng
RT: 8.82 min Scan# 1145
Delta R.T. -0.00 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Instrument :
BNA_F
ClientSampleId :
AOC-7(8)

Tot Ion	Ratio	Resp	Lower	Upper
142	100	254974		
141	86.1	70.5	105.7	
115	53.5	27.7	41.5#	




Manual Integrations
APPROVED


mohammad
9/16/2019 8:59:49 AM

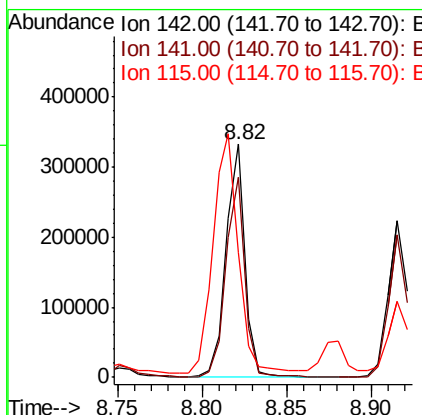

#38
1-Methylnaphthalene
Concen: 19.494 ng
RT: 8.92 min Scan# 1161
Delta R.T. -0.00 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Tgt Ion	Ratio	Resp	Lower	Upper
142	100	178101		
141	90.5	71.9	107.9	
116	8.0	3.2	4.8#	

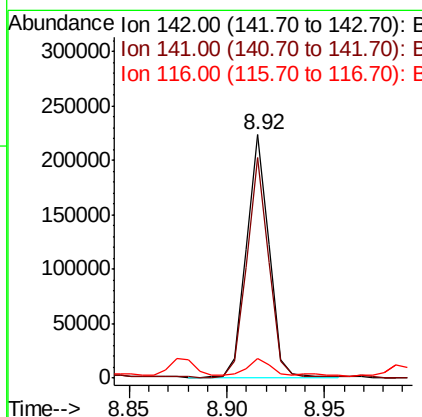







#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.86 min Scan# 1321
Delta R.T. -0.00 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Instrument :
BNA_F
ClientSampleId :
AOC-7-(8)

Tot Ion	Ratio	Resp	Lower	Upper
164	100	167725		
162	104.8	81.8	122.6	
160	45.6	35.7	53.5	




Manual Integrations
APPROVED


mohammad
9/16/2019 8:59:49 AM

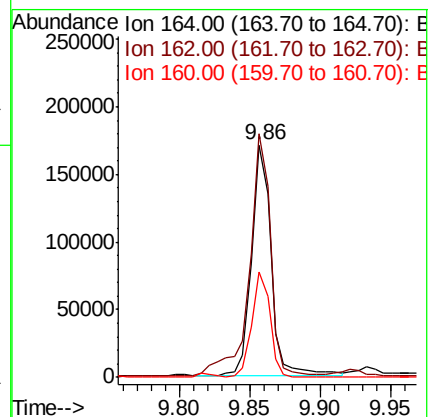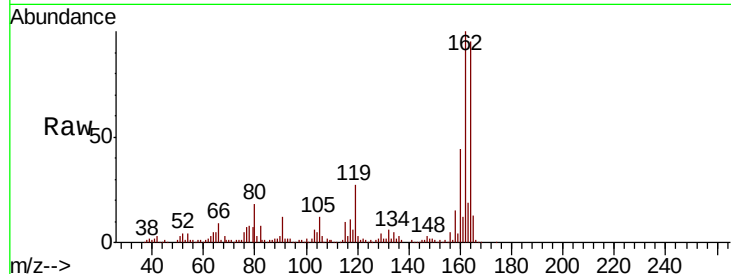

#42
2,4,6-Tribromophenol
Concen: 38.667 ng
RT: 10.64 min Scan# 1454
Delta R.T. -0.01 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Tgt Ion	Ratio	Resp	Lower	Upper
330	100	43356		
332	95.4	75.9	113.9	
141	55.7	35.6	53.4#	

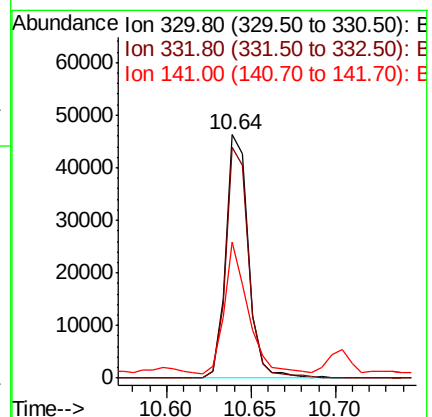







#45
2-Fluorobiphenyl
Concen: 19.471 ng
RT: 9.17 min Scan# 1205
Delta R.T. -0.01 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Instrument :
BNA_F
ClientSampleId :
AOC-7(8)

Tot Ion	Ratio	Resp	Lower	Upper
172	100			
171	34.5	29.1	43.7	
170	23.4	19.2	28.8	




Manual Integrations
APPROVED


mohammad
9/16/2019 8:59:49 AM

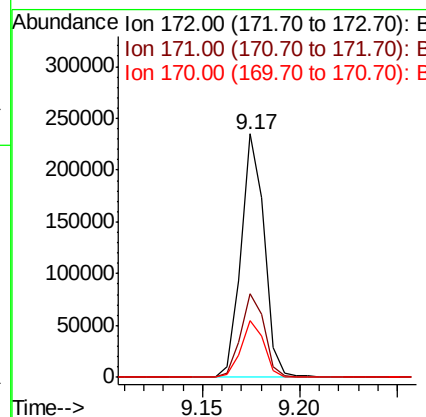

#46
1,1'-Biphenyl
Concen: 3.209 ng
RT: 9.28 min Scan# 1223
Delta R.T. -0.00 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Tgt Ion	Ratio	Resp	Lower	Upper
154	100			
153	40.7	19.8	59.8	
76	13.1	0.0	32.8	

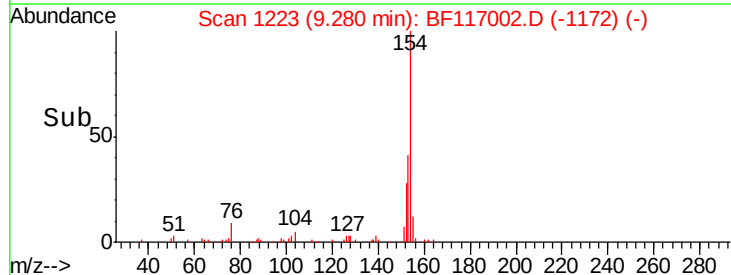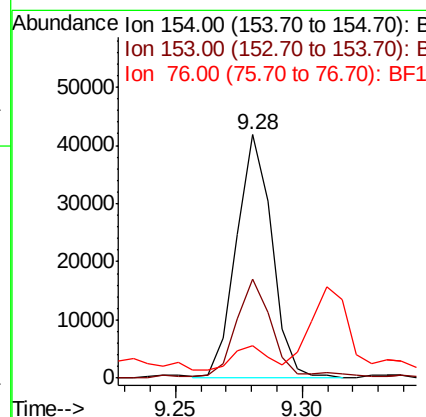







#49
Acenaphthylene
Concen: 15.160 ng
RT: 9.72 min Scan# 1297
Delta R.T. -0.01 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Instrument :
BNA_F
ClientSampleId :
AOC-7(8)

Tot Ion	Ratio	Resp	Lower	Upper
152	100	231004		
151	20.4		16.1	24.1
153	14.2		10.3	15.5




Manual Integrations
APPROVED


mohammad
9/16/2019 8:59:49 AM

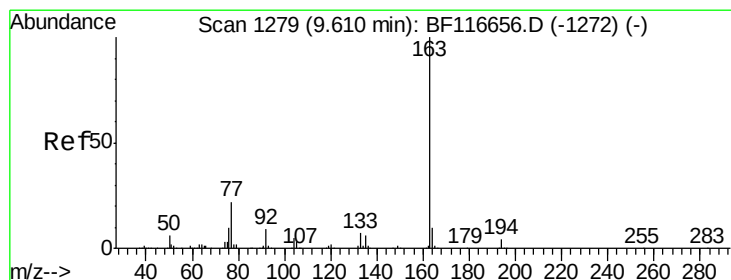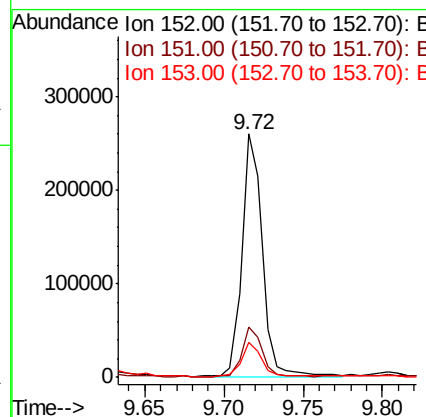

#50
Dimethylphthalate
Concen: 3.444 ng
RT: 9.57 min Scan# 1272
Delta R.T. -0.01 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Tgt Ion	Ratio	Resp	Lower	Upper
163	100	39875		
194	3.6		2.7	4.1
164	34.9		8.2	12.4#

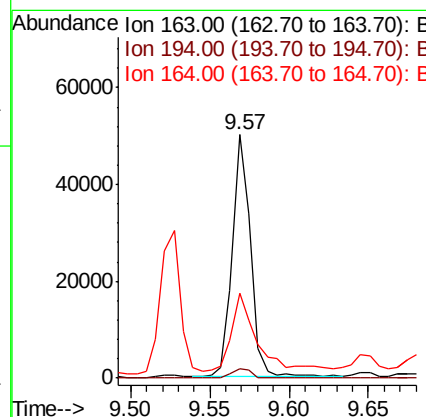

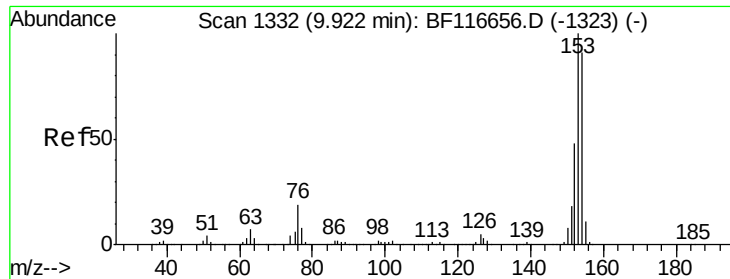

#52

Acenaphthene

Concen: 2.111 ng

RT: 9.89 min Scan# 1327

Delta R.T. -0.00 min

Lab File: BF117002.D

Acq: 12 Sep 2019 19:50

Instrument :

BNA_F


ClientSampleId :

AOC-7(8)

Tot Ion	Ratio	Lower	Upper
154	100		
153	119.6	89.9	134.9
152	74.5	42.6	63.8

Manual Integrations
APPROVED

mohammad
9/16/2019 8:59:49 AM



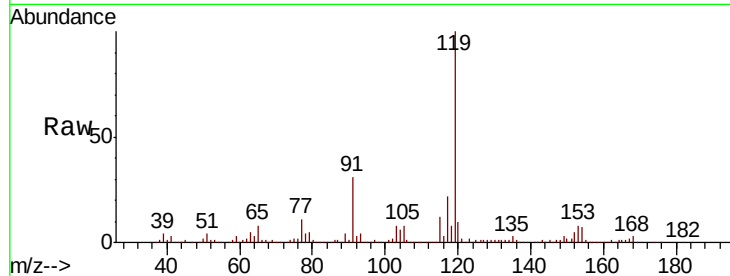


Abundance

Ion 154.00 (153.70 to 154.70): E

Ion 153.00 (152.70 to 153.70): E

Ion 152.00 (151.70 to 152.70): E

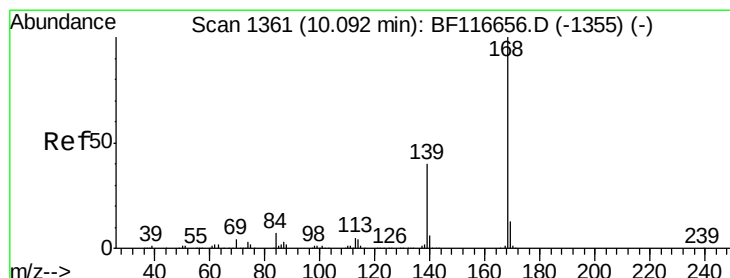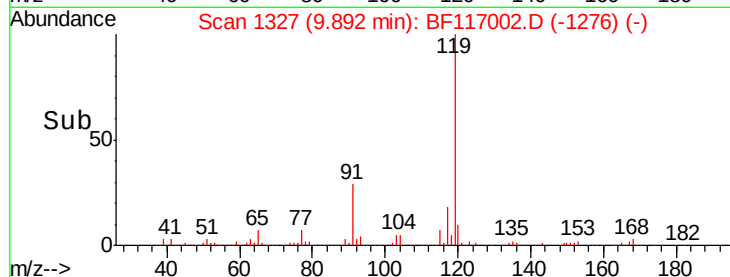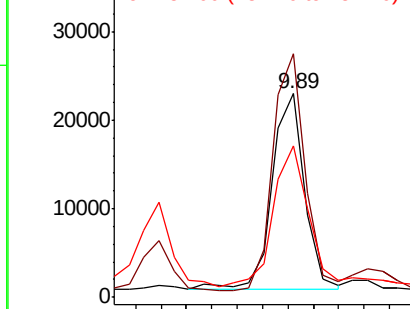

#55

Dibenzofuran

Concen: 2.325 ng

RT: 10.06 min Scan# 1356

Delta R.T. -0.00 min

Lab File: BF117002.D

Acq: 12 Sep 2019 19:50




Tgt Ion	Ratio	Lower	Upper
168	100		
139	38.5	34.2	51.4
169	26.6	11.0	16.4


Abundance

Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 169.00 (168.70 to 169.70): E

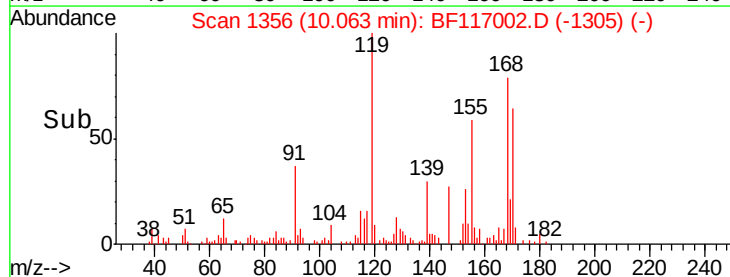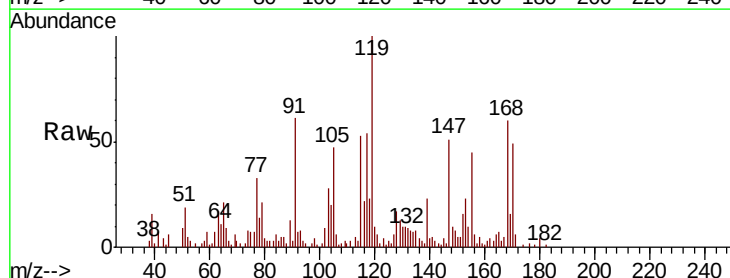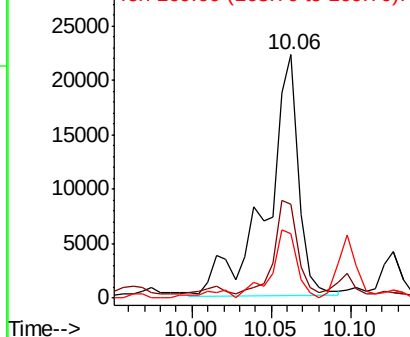







#58
 Fluorene
 Concen: 13.296 ng
 RT: 10.40 min Scan# 1414
 Delta R.T. -0.00 min
 Lab File: BF117002.D
 Acq: 12 Sep 2019 19:50

Instrument :
 BNA_F
 ClientSampleId :
 AOC-7(8)

Tot Ion	Ratio	Lower	Upper
166	100		
165	99.4	77.0	115.6
167	13.5	10.7	16.1




Manual Integrations
 APPROVED


mohammad
 9/16/2019 8:59:49 AM

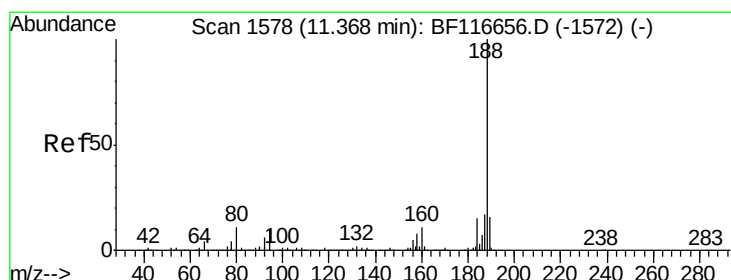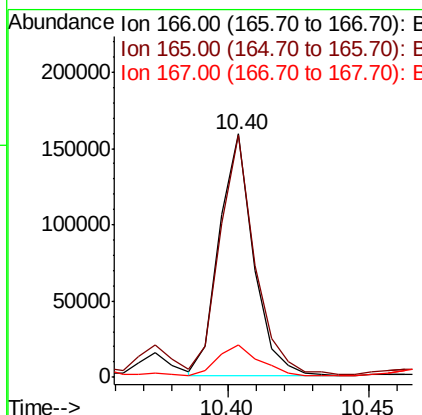

#64
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 11.34 min Scan# 1573
 Delta R.T. -0.00 min
 Lab File: BF117002.D
 Acq: 12 Sep 2019 19:50

Tgt Ion	Ratio	Lower	Upper
188	100		
94	9.2	7.4	11.2
80	10.3	8.5	12.7

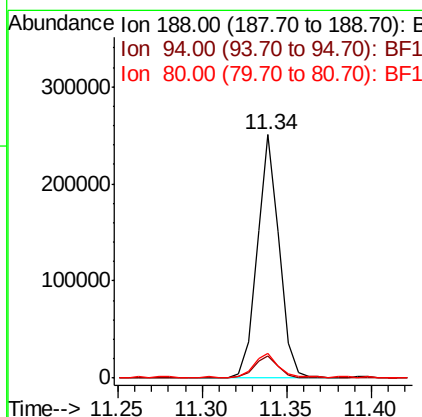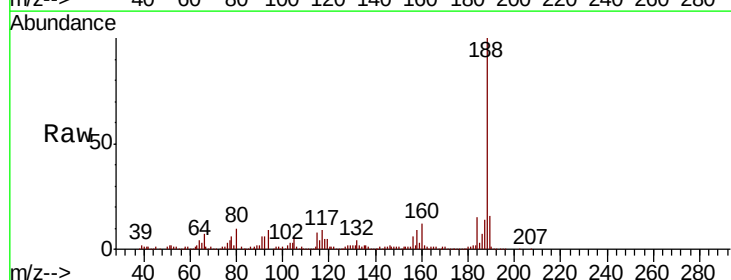







#71
Phenanthrene
Concen: 57.732 ng
RT: 11.37 min Scan# 1578
Delta R.T. -0.00 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Instrument :
BNA_F
ClientSampled :
AOC-7(8)

Tot Ion	Ratio	Lower	Upper
178	100		
176	19.4	15.7	23.5
179	15.5	12.0	18.0




Manual Integrations
APPROVED


mohammad
9/16/2019 8:59:49 AM

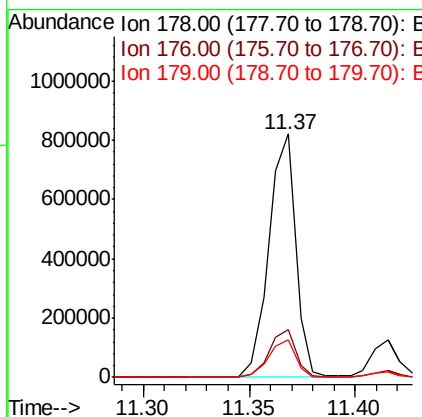

#72
Anthracene
Concen: 8.137 ng
RT: 11.42 min Scan# 1586
Delta R.T. -0.00 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Tgt Ion	Ratio	Lower	Upper
178	100		
176	18.5	15.0	22.6
179	14.8	12.3	18.5

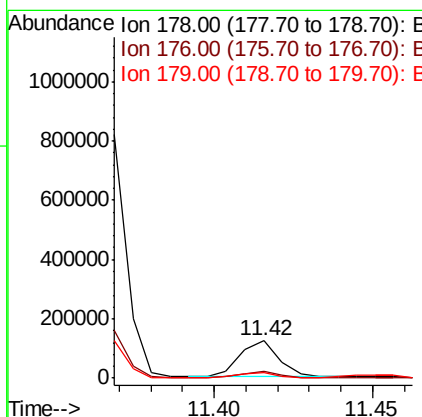



#75

Fluoranthene

Concen: 32.048 ng

RT: 12.56 min Scan# 1780

Delta R.T. 0.01 min

Lab File: BF117002.D

Acq: 12 Sep 2019 19:50

Instrument :

BNA_F


ClientSampled :

AOC-7(8)

Tot Ion	Ion	Ratio	Resp	Lower	Upper
202	100		397886		
101	10.5	0.0	32.0		
203	18.7	0.0	37.5		

Manual Integrations
APPROVED

mohammad
9/16/2019 8:59:49 AM






Abundance

Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 203.00 (202.70 to 203.70): E

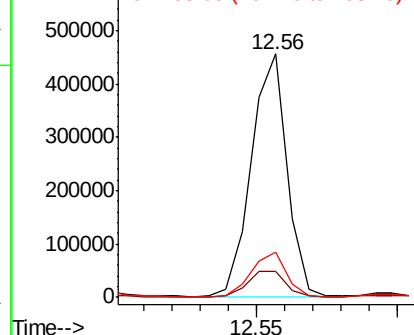

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.98 min Scan# 2022

Delta R.T. 0.01 min

Lab File: BF117002.D

Acq: 12 Sep 2019 19:50




Tgt Ion	Ion	Ratio	Resp	Lower	Upper
240	100		167446		
120	12.4	9.1	13.7		
236	24.4	20.9	31.3		


Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

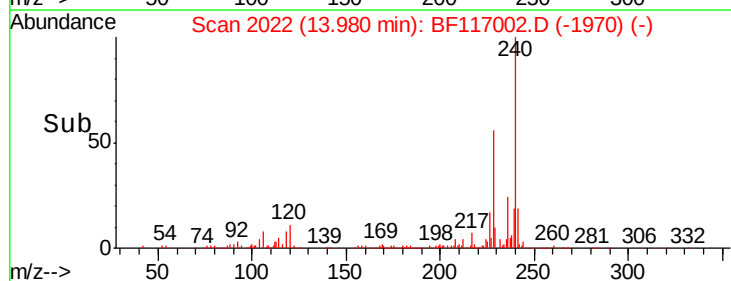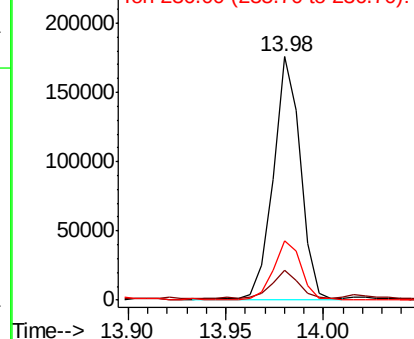



#78

Pvrene

Concen: 43.479 ng

RT: 12.79 min Scan# 1819

Delta R.T. 0.01 min

Lab File: BF117002.D

Acq: 12 Sep 2019 19:50

Instrument :

BNA_F





ClientSampleId :

AOC-7(8)

Tot Ion:	202	Resp:	647179
Ion Ratio		Lower	Upper
202	100		
200	21.3	17.2	25.8
203	17.5	14.2	21.2

Manual Integrations
APPROVED

mohammad
9/16/2019 8:59:49 AM

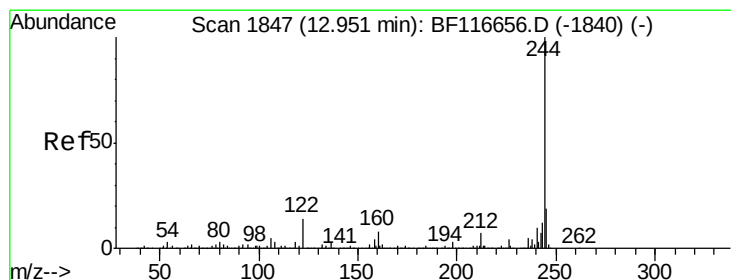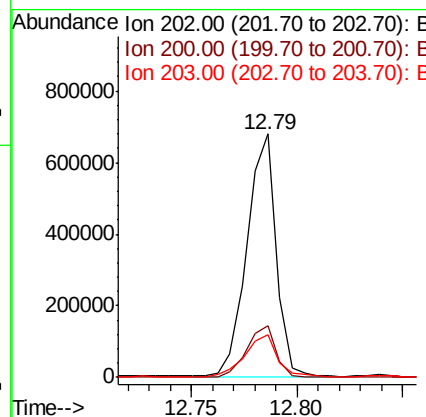

#79

Terphenyl-d14

Concen: 15.547 ng




RT: 12.92 min Scan# 1841


Delta R.T. -0.01 min

Lab File: BF117002.D

Acq: 12 Sep 2019 19:50

Tgt Ion:	244	Resp:	140726
Ion Ratio		Lower	Upper
244	100		
212	6.8	5.7	8.5
122	13.5	11.5	17.3

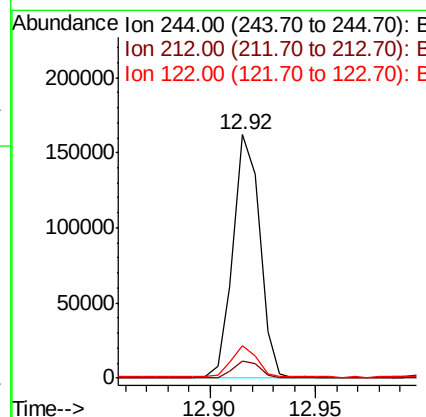



#81

Benzo(a)anthracene

Concen: 27.391 ng

RT: 13.97 min Scan# 2020

Delta R.T. 0.01 min

Lab File: BF117002.D

Acq: 12 Sep 2019 19:50

Instrument :

BNA_F


ClientSampleId :

AOC-7(8)




Tot Ion:	228	Resp:	290280
Ion Ratio	Lower	Upper	
228	100		
226	28.6	22.3	33.5
229	20.7	15.8	23.8

Manual Integrations
APPROVED

mohammad
9/16/2019 8:59:49 AM



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

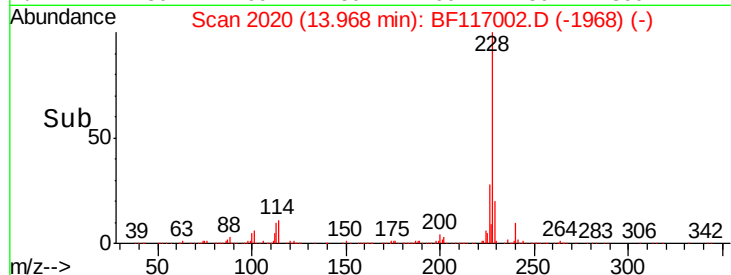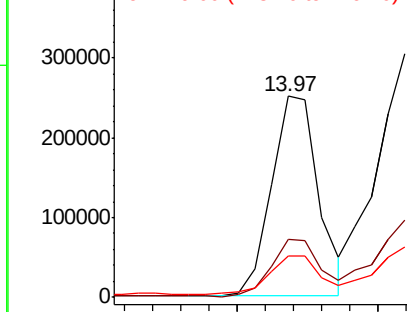

#83

Chrysene

Concen: 29.025 ng


RT: 14.01 min Scan# 2027

Delta R.T. 0.01 min



Lab File: BF117002.D


Acq: 12 Sep 2019 19:50

Tgt Ion:	228	Resp:	316904
Ion Ratio	Lower	Upper	
228	100		
226	31.9	24.5	36.7
229	20.6	15.7	23.5



Abundance Ion 228.00 (227.70 to 228.70): E
Ion 226.00 (225.70 to 226.70): E
Ion 229.00 (228.70 to 229.70): E

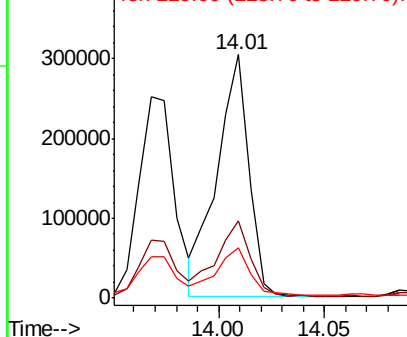




#86
 Indeno(1,2,3-cd)pyrene
 Concen: 9.700 ng
 RT: 16.87 min Scan# 2513
 Delta R.T. 0.01 min
 Lab File: BF117002.D
 Acq: 12 Sep 2019 19:50

Instrument :
 BNA_F
 ClientSampleId :
 AOC-7(8)

Tot Ion	Ratio	Lower	Upper
276	100		
138	21.4	20.6	31.0
277	24.0	19.9	29.9

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:59:49 AM






Abundance

Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 277.00 (276.70 to 277.70): E

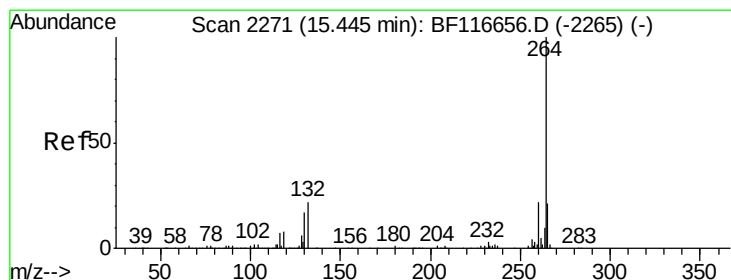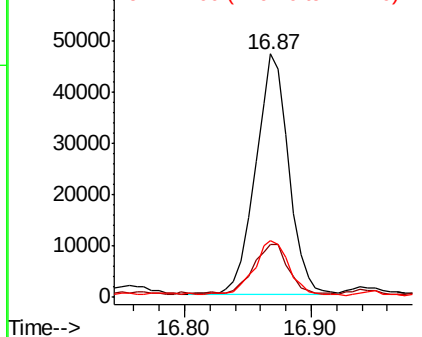

#87
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.44 min Scan# 2270
 Delta R.T. 0.02 min
 Lab File: BF117002.D
 Acq: 12 Sep 2019 19:50




Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.9	19.0	28.4
265	23.5	17.9	26.9


Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

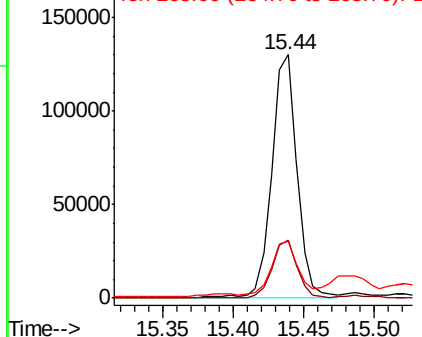

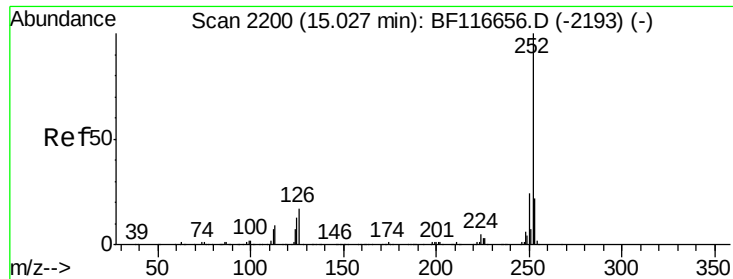





#88
Benzo(b)fluoranthene
Concen: 25.494 ng m
RT: 15.02 min Scan# 2199
Delta R.T. 0.02 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Instrument :
BNA_F
ClientSampleId :
AOC-7(8)

Tot Ion	Ratio	Lower	Upper
252	100		
253	21.7	17.5	26.3
125	12.0	8.3	12.5




Manual Integrations
APPROVED


mohammad
9/16/2019 8:59:49 AM

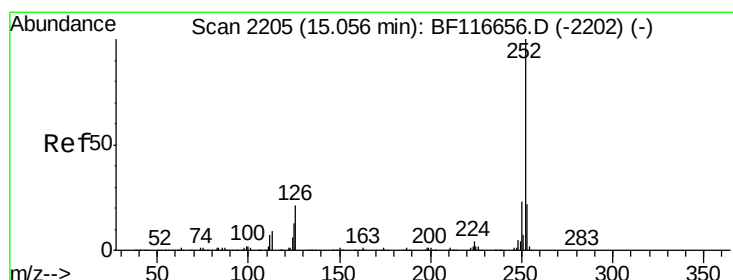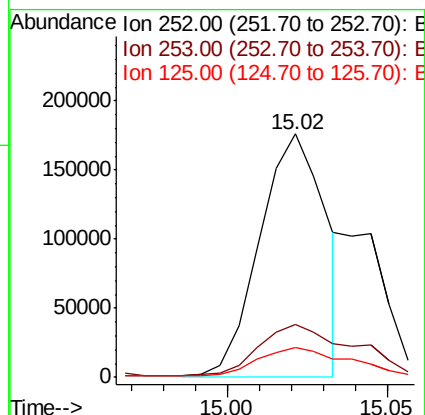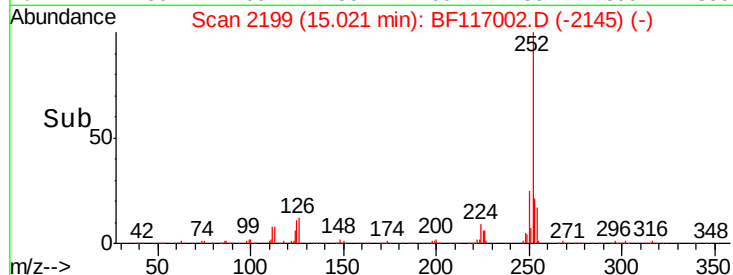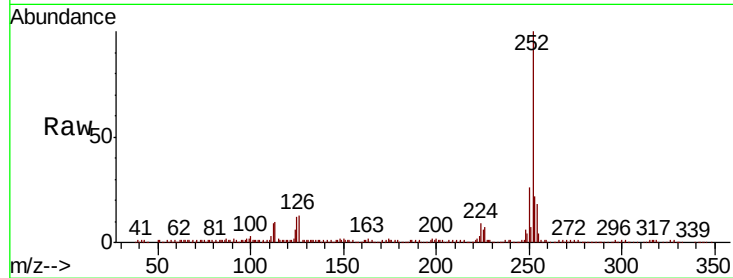

#89
Benzo(k)fluoranthene
Concen: 10.781 ng m
RT: 15.03 min Scan# 2201
Delta R.T. -0.00 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Tgt Ion	Ratio	Lower	Upper
252	100		
253	23.5	16.8	25.2
125	12.8	7.6	11.4#

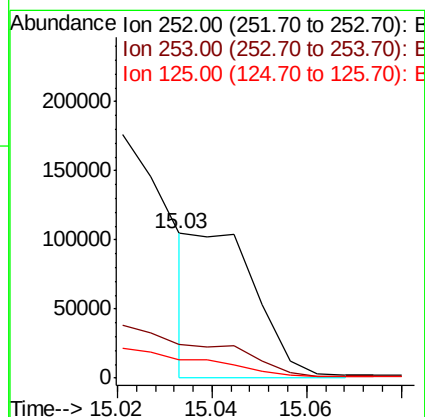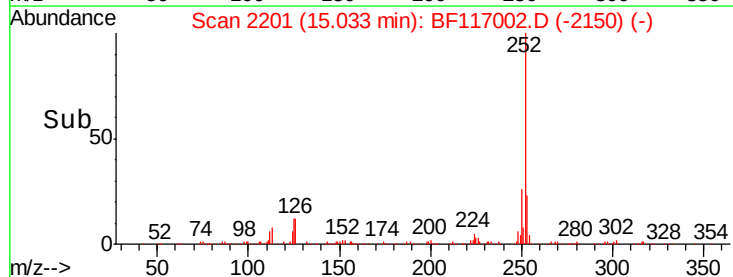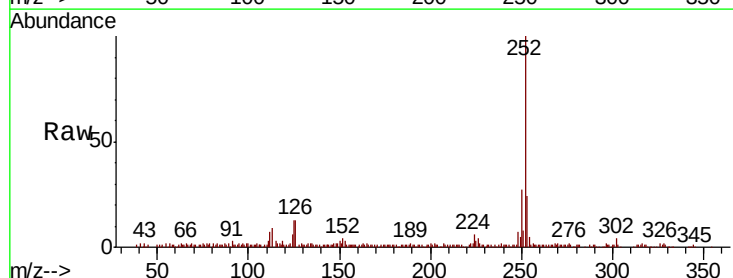




#90
Benzo(a)pyrene
Concen: 17.977 ng
RT: 15.37 min Scan# 2259
Delta R.T. 0.02 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Instrument :
BNA_F
ClientSampled :
AOC-7(8)

Tot Ion	Ratio	Resp	Lower	Upper
252	100	155549		
253	22.3		17.6	26.4
125	12.2		10.2	15.2

Manual Integrations
APPROVED

mohammad
9/16/2019 8:59:49 AM






Abundance

Ion 252.00 (251.70 to 252.70): E


Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

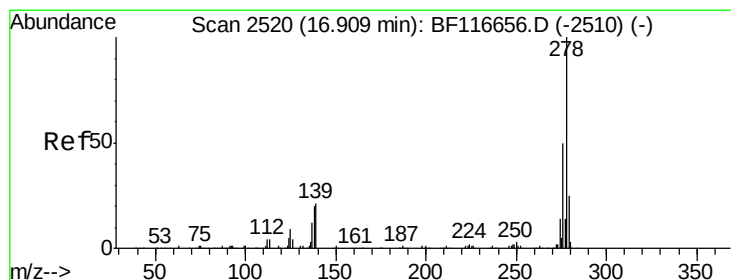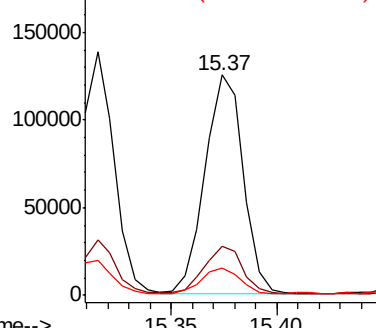

#91
Dibenzo(a,h)anthracene
Concen: 3.738 ng m
RT: 16.87 min Scan# 2514
Delta R.T. 0.01 min
Lab File: BF117002.D
Acq: 12 Sep 2019 19:50

Tgt Ion	Ratio	Resp	Lower	Upper
278	100	28309		
139	20.8		13.1	19.7#
279	27.1		18.6	27.8






Abundance

Ion 278.00 (277.70 to 278.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 279.00 (278.70 to 279.70): E

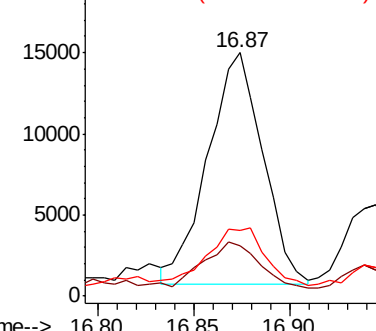



#92
 Benzo(a,h,i)perylene
 Concen: 10.229 ng
 RT: 17.30 min Scan# 2587
 Delta R.T. 0.02 min
 Lab File: BF117002.D
 Acq: 12 Sep 2019 19:50

Instrument :
 BNA_F
 ClientSampleId :
 AOC-7(8)

Tot Ion:	276	Resp:	79011
Ion Ratio	Lower	Upper	
276	100		
277	23.3	19.0	28.6
138	18.9	18.7	28.1

Manual Integrations
 APPROVED

mohammad
 9/16/2019 8:59:49 AM

