

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091219\
 Data File : BF117005.D
 Acq On : 12 Sep 2019 21:10
 Operator : HP/JU
 Sample : K4825-12 5X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CSA-4-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.445	568	571	577	rBV	8460	13133	2.23%	0.443%
2	6.457	741	743	752	rBV	8484	14765	2.51%	0.498%
3	6.598	764	767	772	rBV	16257	19195	3.26%	0.647%
4	6.828	802	806	818	rBV	337782	348896	59.23%	11.768%
5	6.981	829	832	840	rBV	20613	22518	3.82%	0.759%
6	7.392	900	902	912	rBV2	5249	9389	1.59%	0.317%
7	8.104	1020	1023	1046	rBV	444742	503980	85.56%	16.998%
8	9.181	1203	1206	1214	rBV	18744	26983	4.58%	0.910%
9	9.857	1317	1321	1341	rBV	524186	589021	100.00%	19.867%
10	10.645	1452	1455	1461	rBB	6933	8770	1.49%	0.296%
11	11.339	1569	1573	1586	rBV	482347	539053	91.52%	18.181%
12	12.739	1807	1811	1813	rBV4	6537	6214	1.05%	0.210%
13	12.916	1838	1841	1844	rBV	35371	32319	5.49%	1.090%
14	13.363	1914	1917	1921	rVB5	11374	14150	2.40%	0.477%
15	13.968	2017	2020	2028	rBV	398134	432967	73.51%	14.603%
16	15.421	2263	2267	2275	rVB	265425	383500	65.11%	12.935%


Sum of corrected areas: 2964853

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091219\
Data File : BF117005.D
Acq On : 12 Sep 2019 21:10
Operator : HP/JU
Sample : K4825-12 5X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CSA-4-3

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

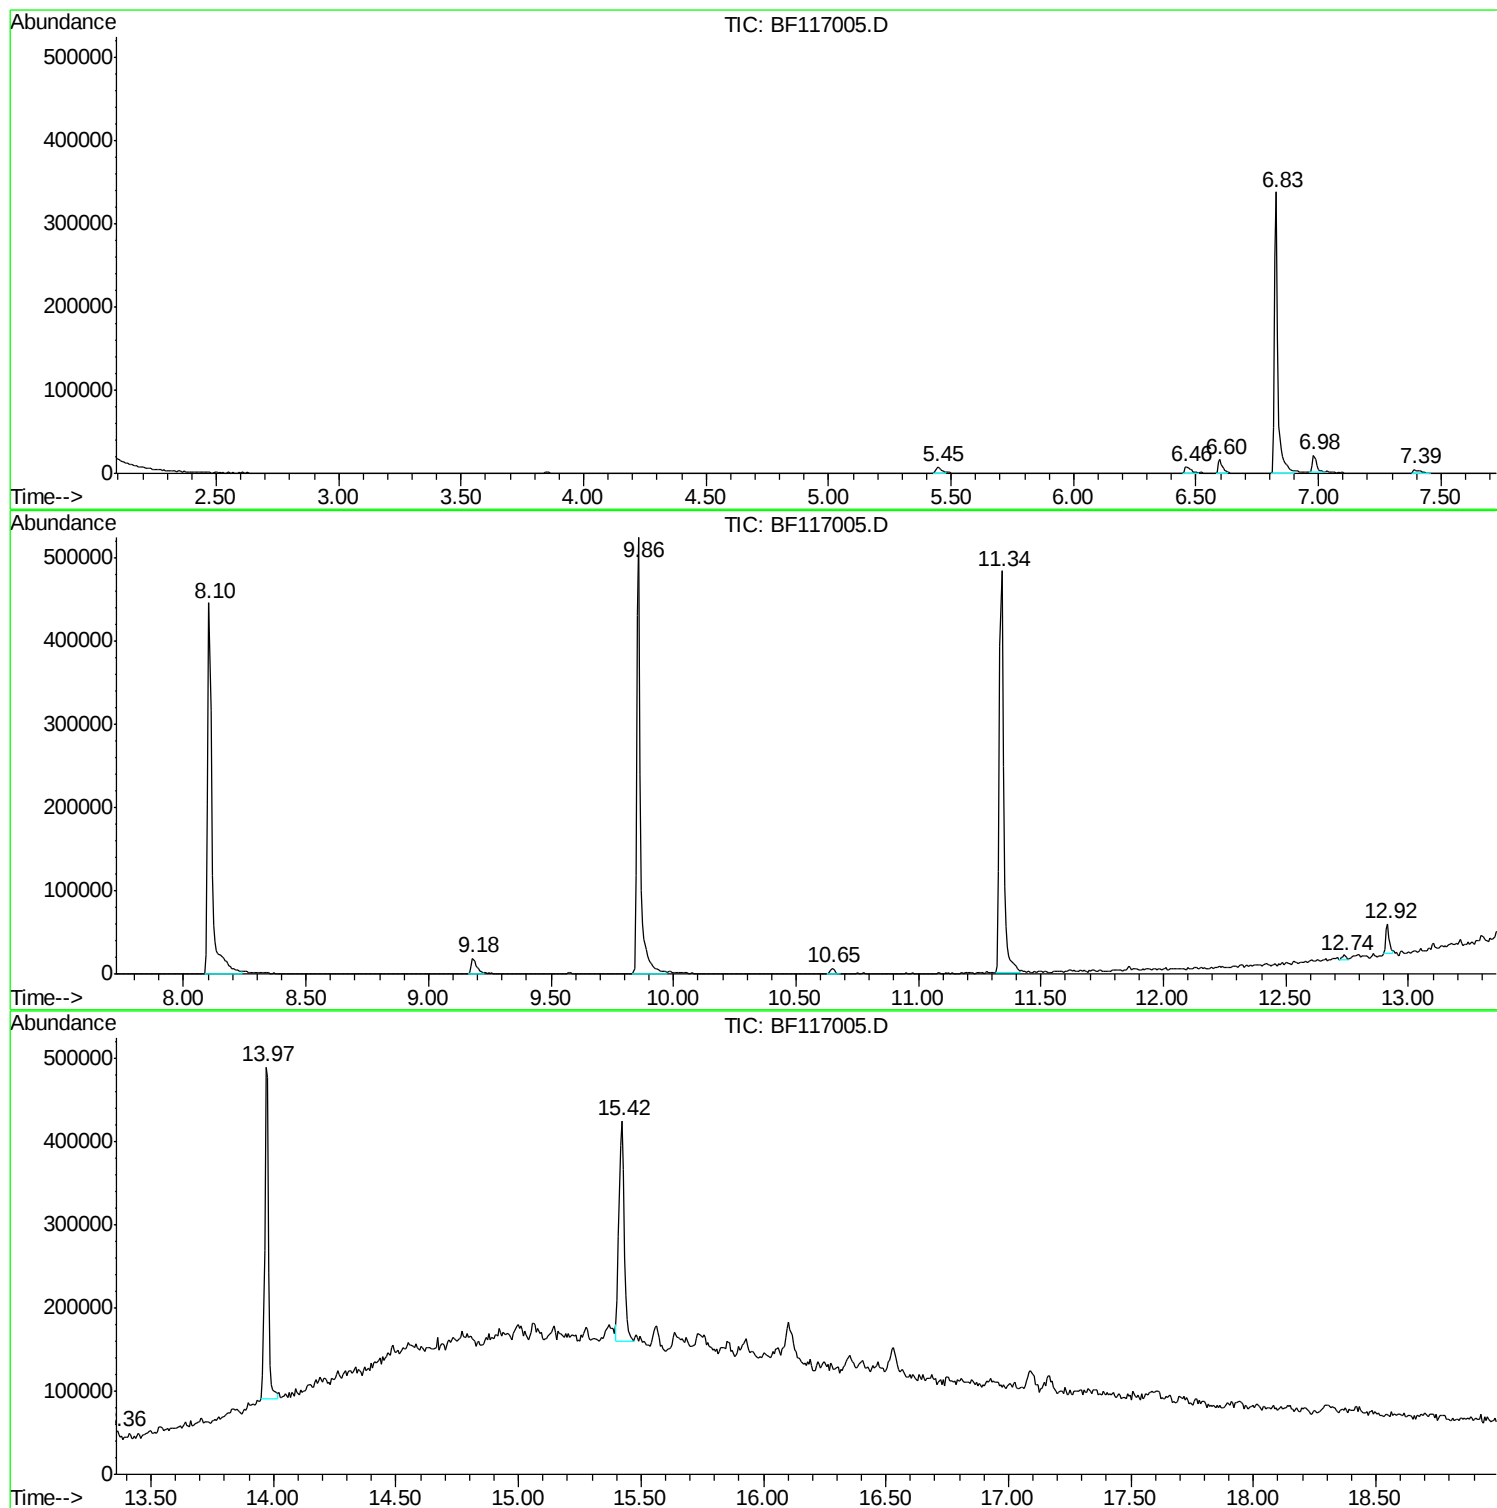

Data_Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091219\
Data_File : BF117005.D
Acq_On : 12-Sep-2019 21:100
Operator : HP/JUU
Sample : K4825-12_5XX
Misc :
ALS_Vial : 25 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
CSA-4-3

Quant_Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATIONN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
