

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091219\
Data File : BF117015.D
Acq On : 13 Sep 2019 9:57
Operator : HP/JU
Sample : PB122992BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB122992BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.445	566	571	574	rBV	1563106	1429210	64.01%	9.244%
2	6.463	739	744	762	rBV	1469589	1611426	72.18%	10.422%
3	6.598	762	767	770	rBV	1874088	1651039	73.95%	10.679%
4	6.828	802	806	818	rVB	415115	375282	16.81%	2.427%
5	6.981	828	832	836	rBV	1406699	1261262	56.49%	8.158%
6	7.386	896	901	920	rBV	1054719	1016849	45.54%	6.577%
7	8.104	1020	1023	1039	rBV	460690	501767	22.47%	3.245%
8	9.180	1201	1206	1221	rBV	1984904	2076000	92.98%	13.427%
9	9.857	1317	1321	1335	rBV	564025	616121	27.60%	3.985%
10	10.639	1450	1454	1472	rBV	1022790	1171480	52.47%	7.577%
11	11.339	1569	1573	1593	rBV	536757	636896	28.53%	4.119%
12	12.915	1837	1841	1856	rBV	2282782	2232643	100.00%	14.440%
13	13.968	2016	2020	2035	rBV	400703	497977	22.30%	3.221%
14	15.421	2261	2267	2278	rBV	207507	383370	17.17%	2.480%


Sum of corrected areas: 15461322

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091219\
Data File : BF117015.D
Acq On : 13 Sep 2019 9:57
Operator : HP/JU
Sample : PB122992BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB122992BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

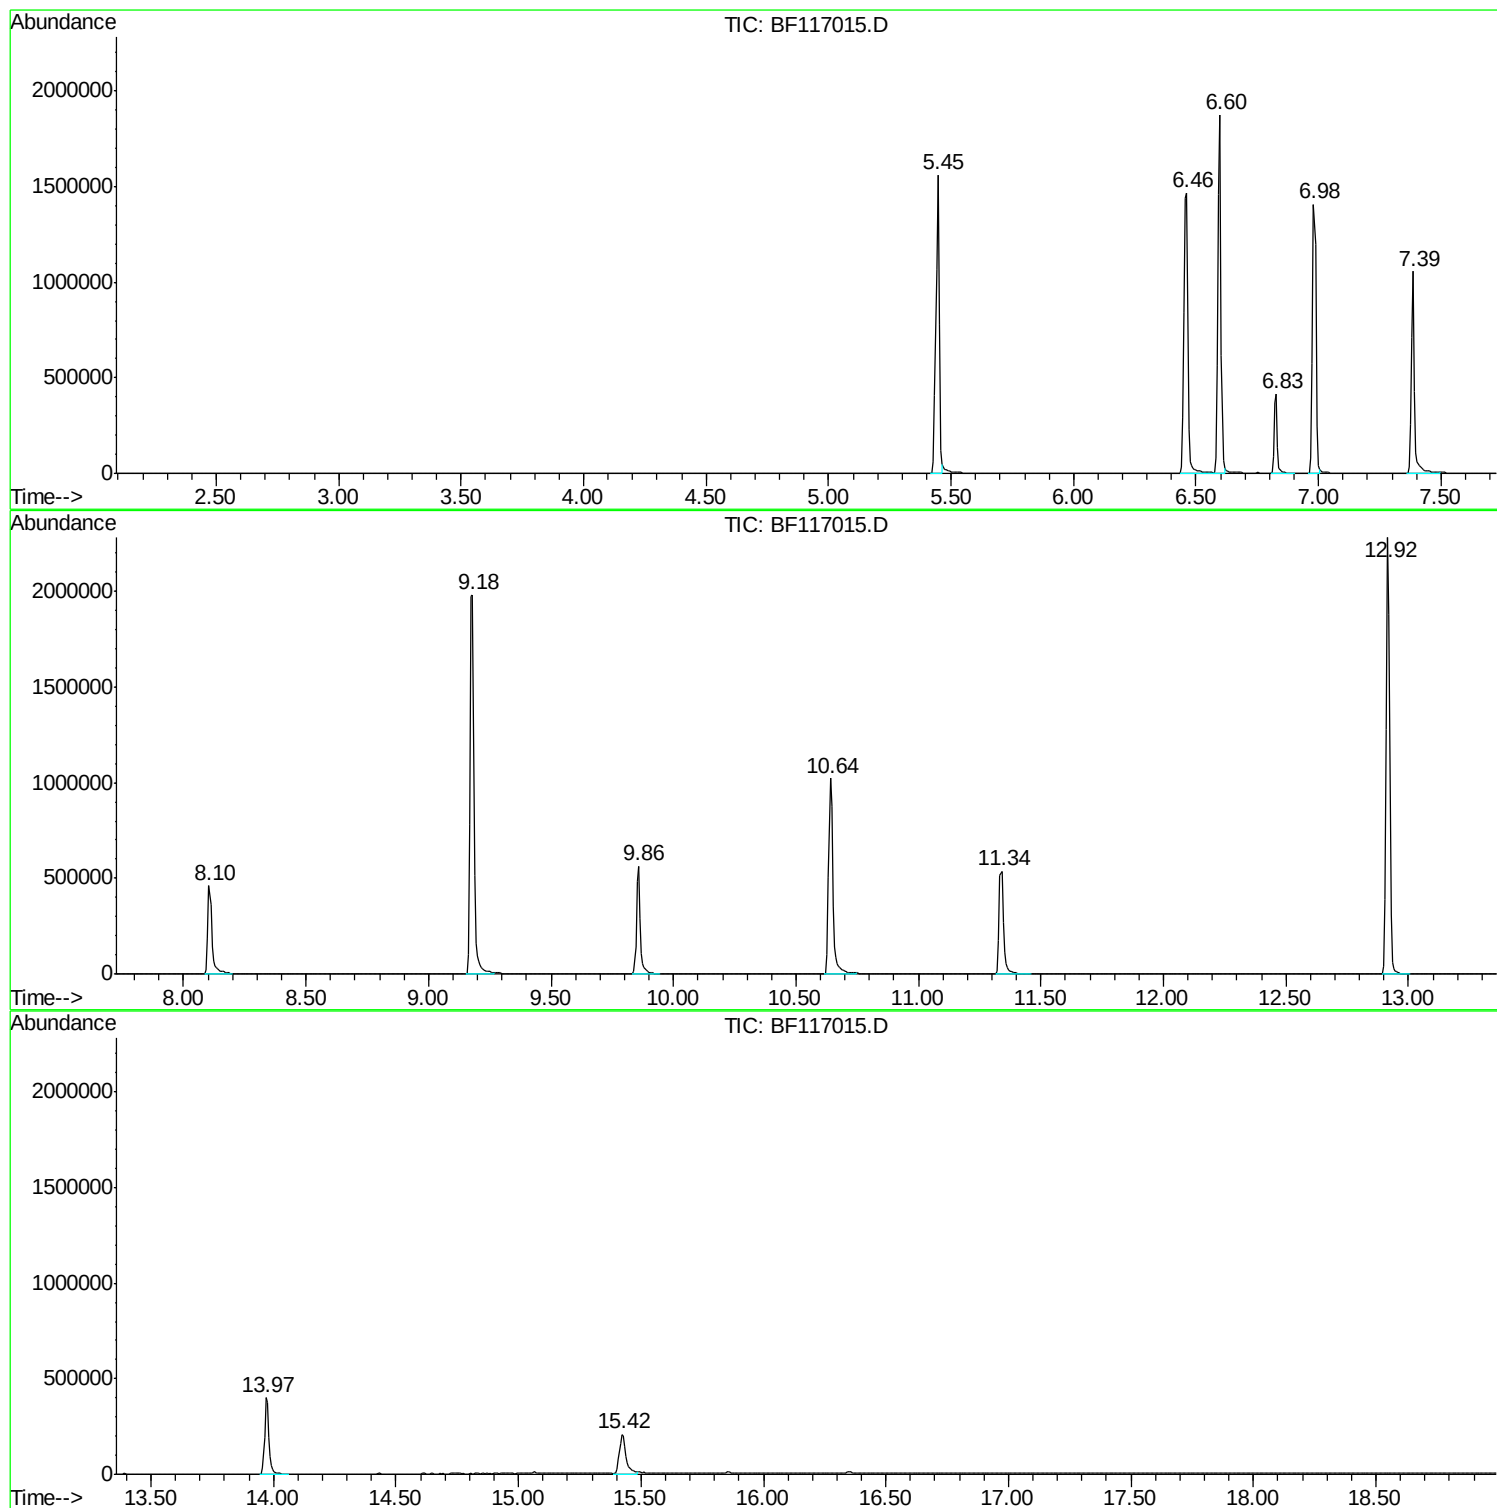

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF091219\
Data File : BF117015.D
Acq On : 13 Sep 2019 9:57
Operator : HP/JU
Sample : PB122992BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB122992BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.60	87.99 ng	1651040	1,4-Dichlorobenzene-d4	6.83

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

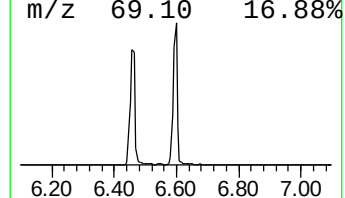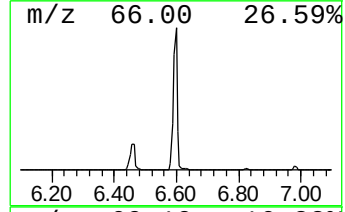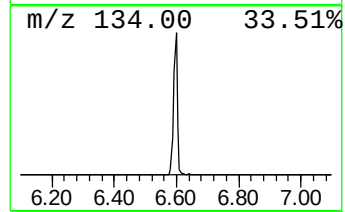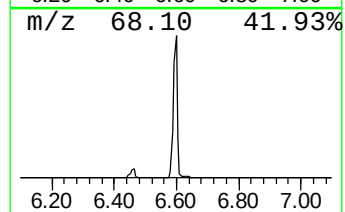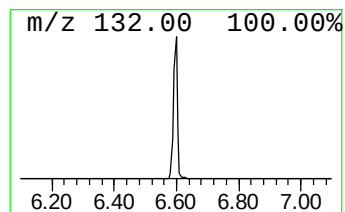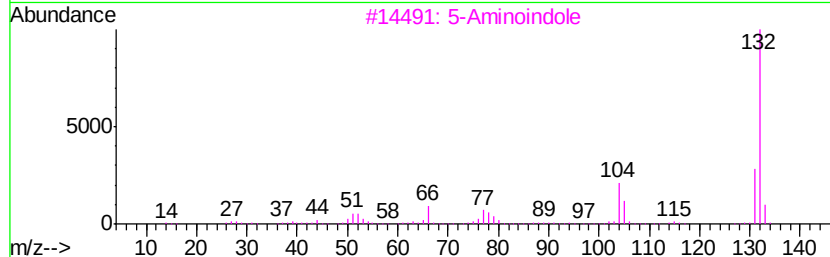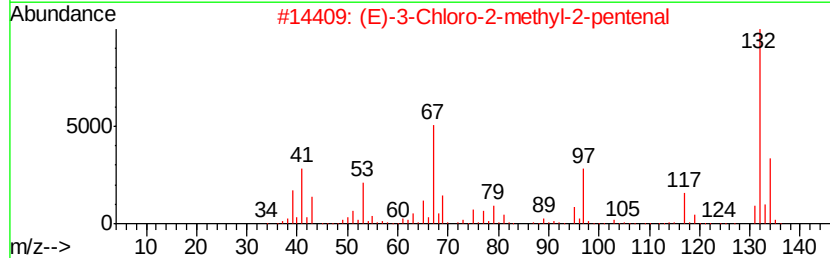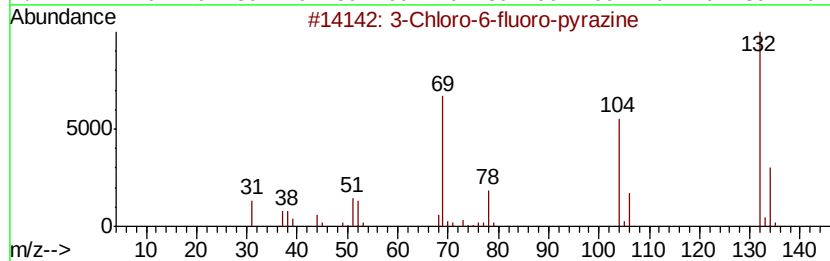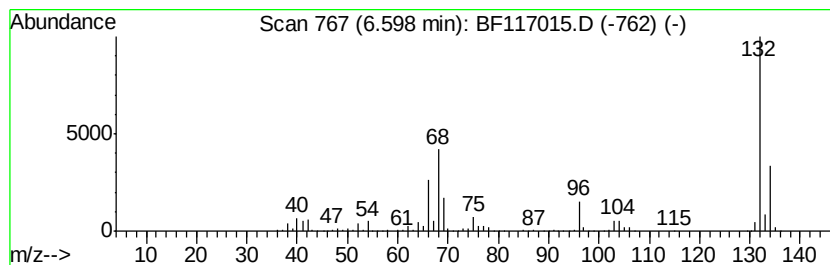

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091219\
Data File : BF117015.D
Acq On : 13 Sep 2019 9:57
Operator : HP/JU
Sample : PB122992BL
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB122992BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.60	6.60	88.0	ng	1651040	1	6.83	375282	20.0