


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF091219\  
 Data File : BF116981.D  
 Acq On : 12 Sep 2019 9:45  
 Operator : HP/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF083019.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Sep 12 08:24:39 2019

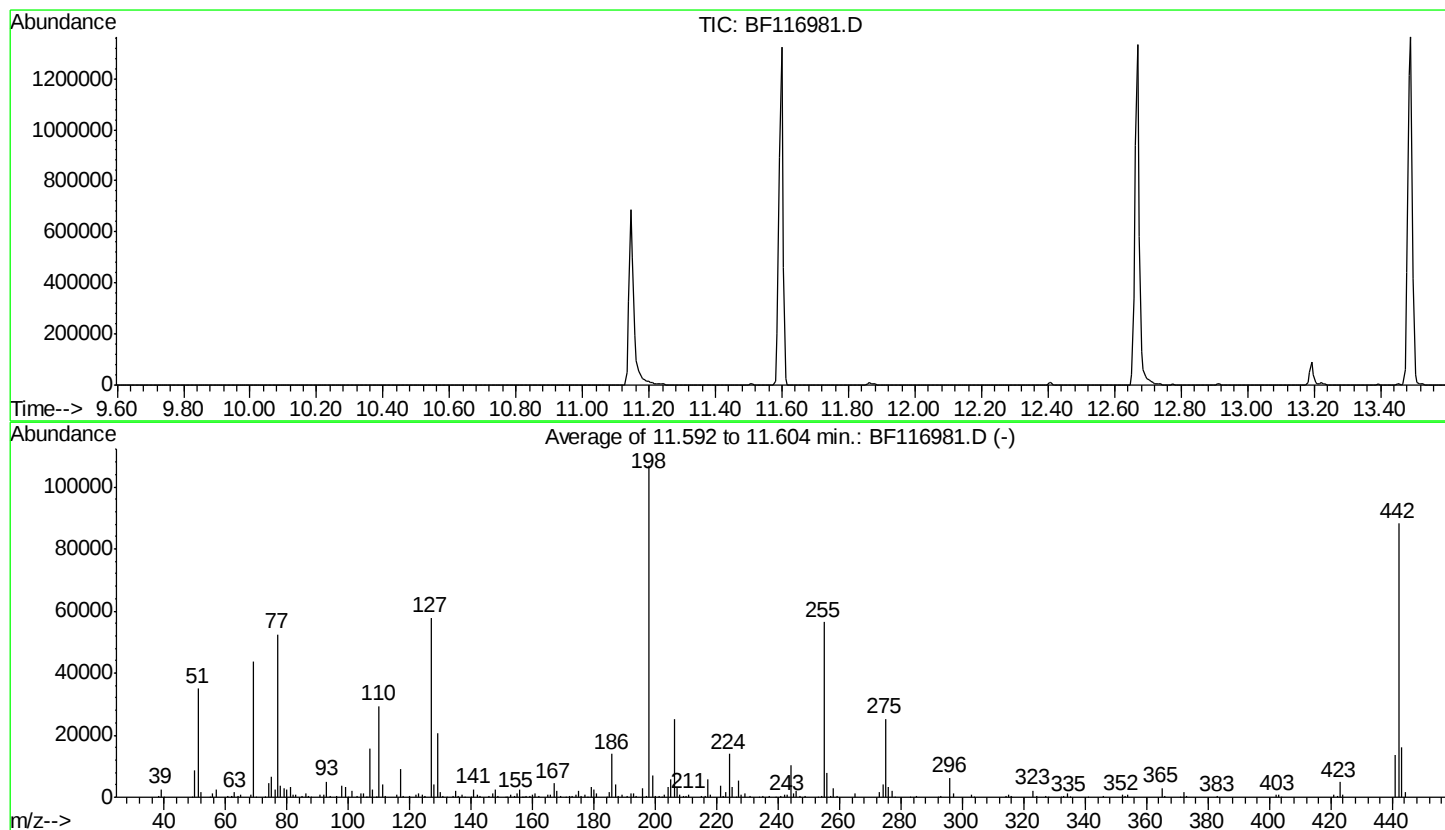

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 32.7      | 34875   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 681     | PASS             |
| 69          | 198          | 0.00         | 100          | 41.0      | 43784   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 121     | PASS             |
| 127         | 198          | 10           | 80           | 54.2      | 57906   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 607     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 106813  | PASS             |
| 199         | 198          | 5            | 9            | 6.4       | 6888    | PASS             |
| 275         | 198          | 10           | 60           | 23.6      | 25230   | PASS             |
| 365         | 198          | 1            | 100          | 2.9       | 3050    | PASS             |
| 441         | 198          | 0.01         | 100          | 12.8      | 13655   | PASS             |
| 442         | 198          | 50           | 100          | 82.4      | 88064   | PASS             |
| 443         | 442          | 15           | 24           | 18.3      | 16092   | PASS             |