


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF091219\
 Data File : BF117006.D
 Acq On : 12 Sep 2019 22:31
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF083019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Sep 12 08:24:39 2019

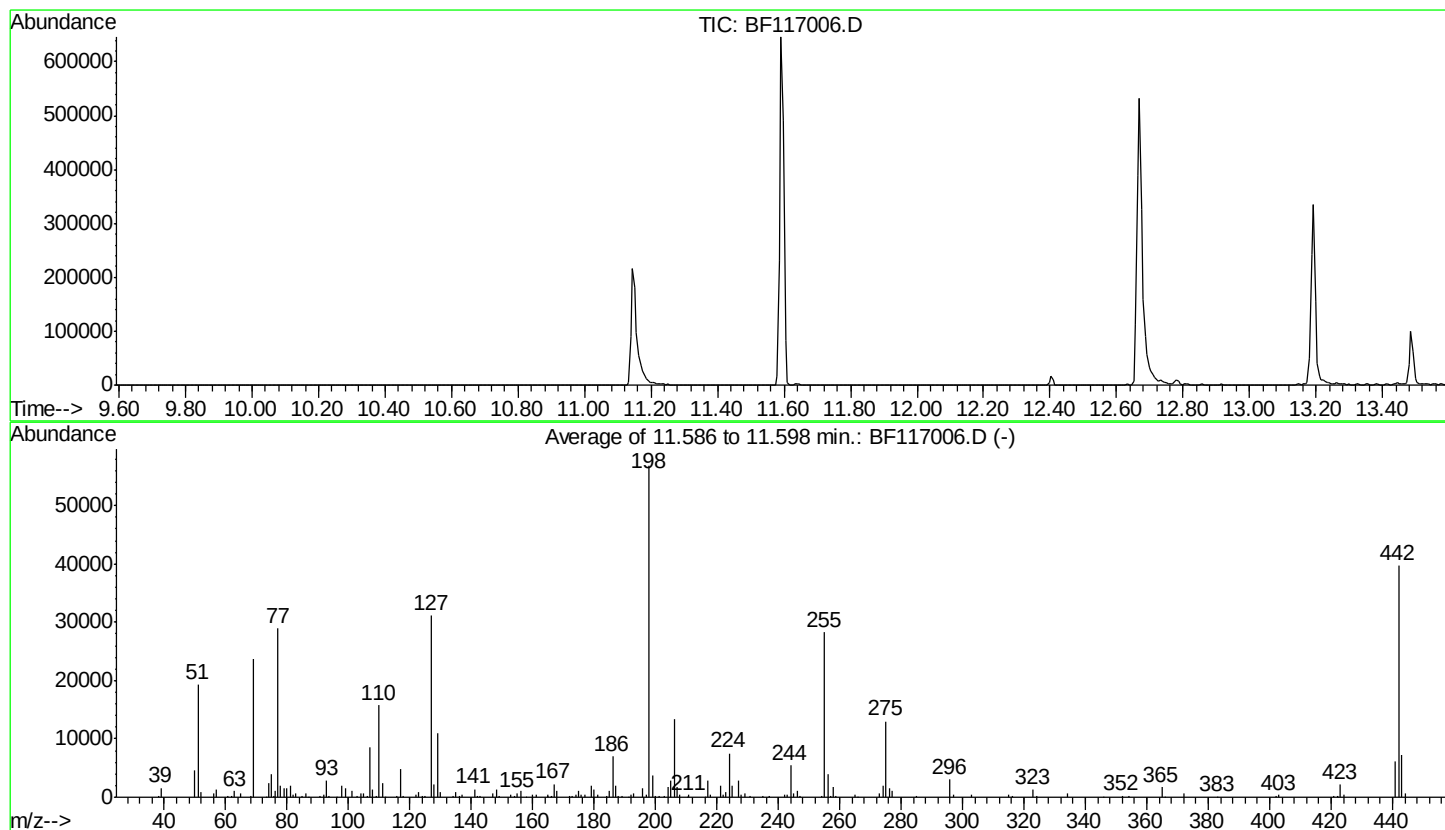

AutoFind: Scans 1615, 1616, 1617; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	19288	PASS
68	69	0.00	2	1.0	238	PASS
69	198	0.00	100	41.6	23648	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.7	31074	PASS
197	198	0.00	2	0.6	365	PASS
198	198	100	100	100.0	56858	PASS
199	198	5	9	6.6	3764	PASS
275	198	10	60	22.9	13004	PASS
365	198	1	100	2.9	1655	PASS
441	198	0.01	100	10.8	6146	PASS
442	198	50	100	69.7	39646	PASS
443	442	15	24	18.0	7149	PASS