
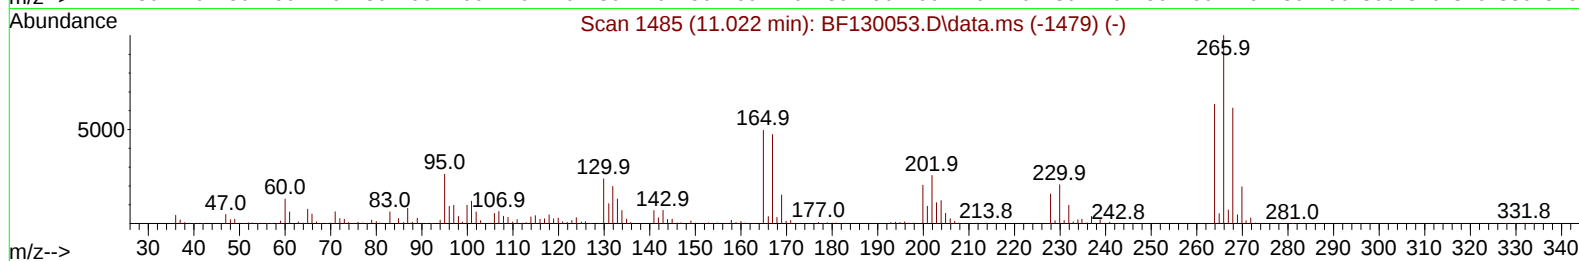
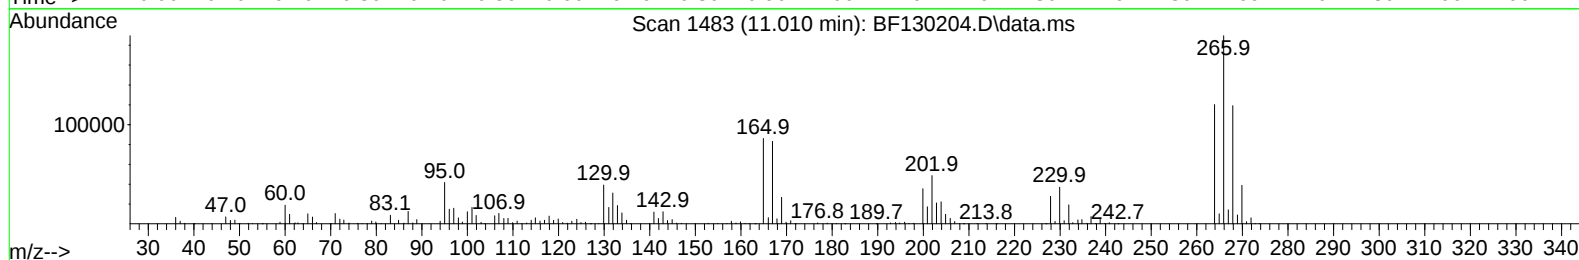


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF091222\  
Data File : BF130204.D  
Acq On : 12 Sep 2022 10:52  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 05:42:07 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF083122.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 07 02:05:07 2022  
Response via : Initial Calibration

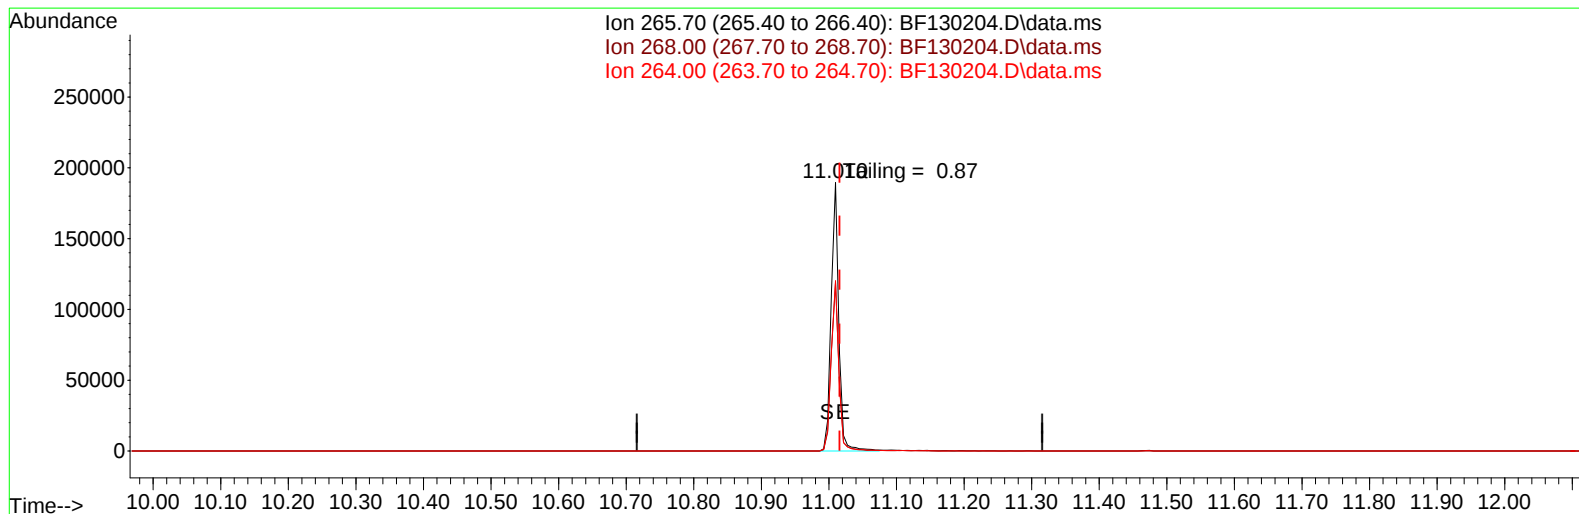

TIC: BF130204.D\data.ms

**(70) Pentachlorophenol (C)**




11.010min (-0.006) 26910.92 ng

response 150285

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.20  | 62.81  |
| 264.00 | 59.90  | 63.42  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF091222\  
Data File : BF130204.D  
Acq On : 12 Sep 2022 10:52  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 13 05:42:07 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF083122.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 07 02:05:07 2022  
Response via : Initial Calibration

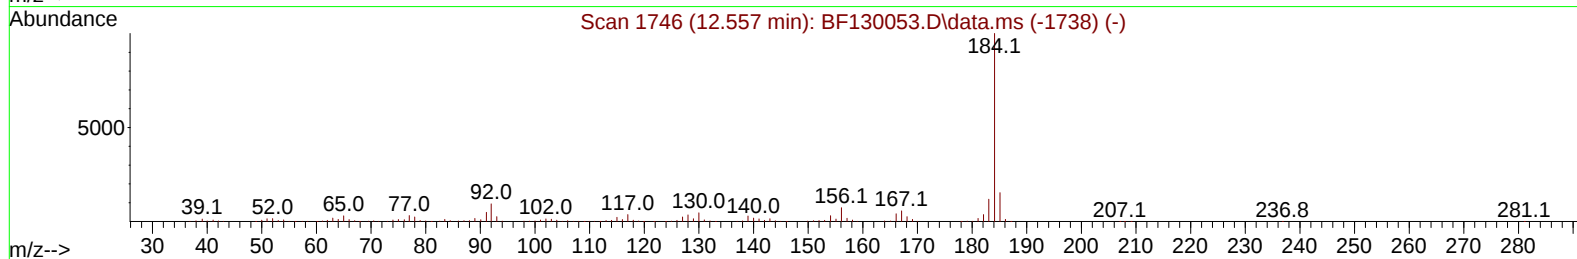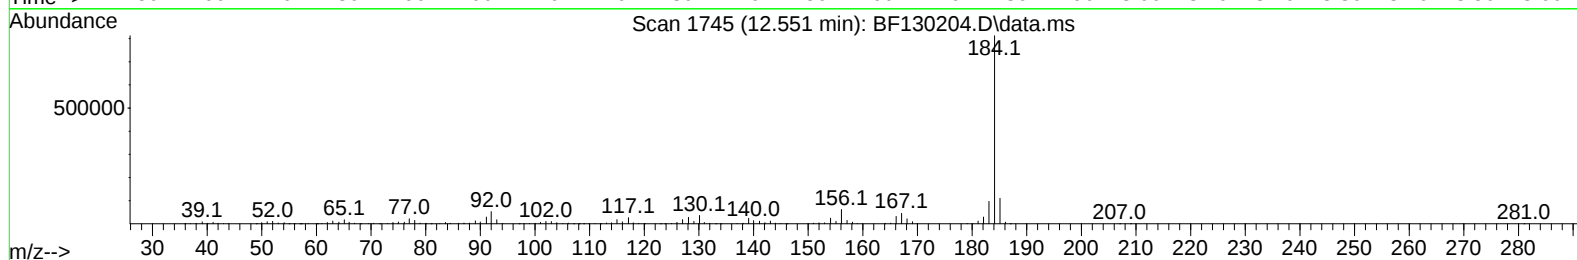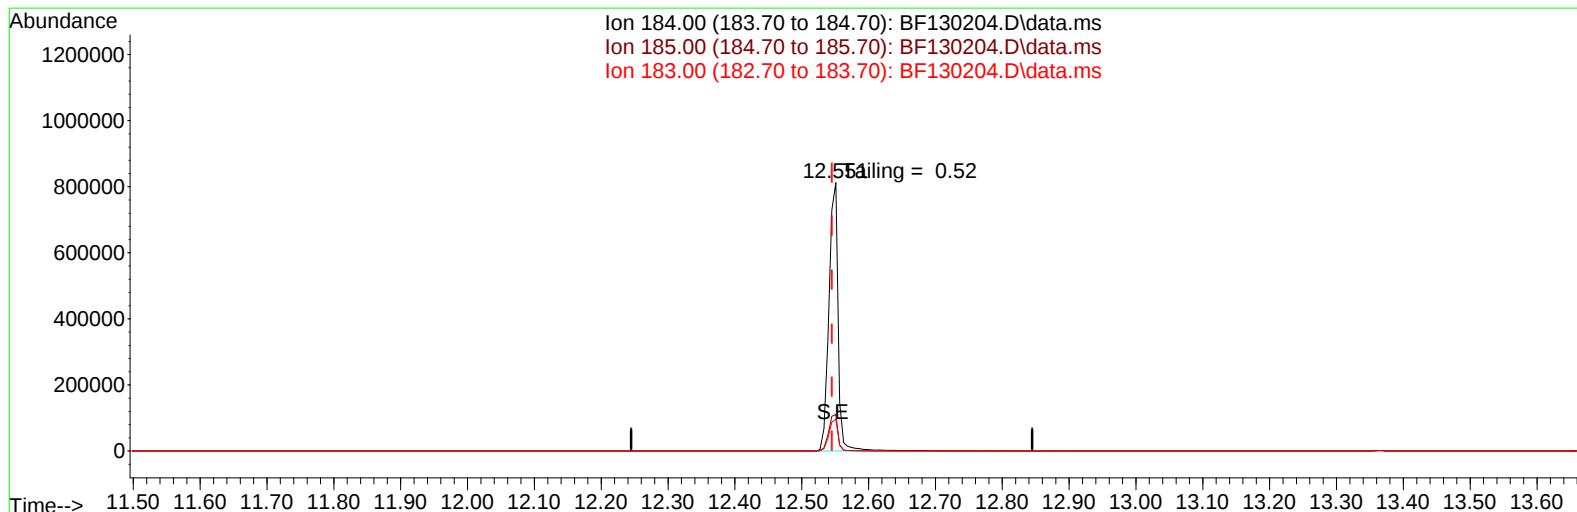

TIC: BF130204.D\data.ms

**(77) Benzidine**

12.551min (+ 0.006) 0.00 ng

response 774051

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.30  | 13.58  |
| 183.00 | 11.80  | 11.90  |
| 0.00   | 0.00   | 0.00   |