

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
 Data File : BF130210.D
 Acq On : 12 Sep 2022 17:57
 Operator : CG\JU
 Sample : N4551-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 251032-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130210.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.863	435	438	446	rVB	40659	45486	1.39%	0.280%
2	5.281	505	509	513	rBV	1429268	1238834	37.91%	7.621%
3	6.310	680	684	693	rBV	926949	732555	22.42%	4.506%
4	6.687	744	748	751	rBV	810359	625649	19.15%	3.849%
5	7.251	839	844	847	rBV	2198649	1888477	57.80%	11.617%
6	7.969	962	966	969	rBV	970119	800506	24.50%	4.924%
7	9.045	1144	1149	1152	rBV	4072679	3267441	100.00%	20.100%
8	9.716	1259	1263	1266	rBV	1080706	810911	24.82%	4.988%
9	10.504	1392	1397	1400	rBV	2088347	1797588	55.02%	11.058%
10	11.198	1511	1515	1518	rBV	875880	689102	21.09%	4.239%
11	12.786	1780	1785	1788	rBV	3037891	2796801	85.60%	17.205%
12	13.827	1958	1962	1965	rBV	777408	716742	21.94%	4.409%
13	15.221	2194	2199	2206	rBV	711746	845868	25.89%	5.203%




Sum of corrected areas: 16255960

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
Data File : BF130210.D
Acq On : 12 Sep 2022 17:57
Operator : CG\JU
Sample : N4551-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
251032-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

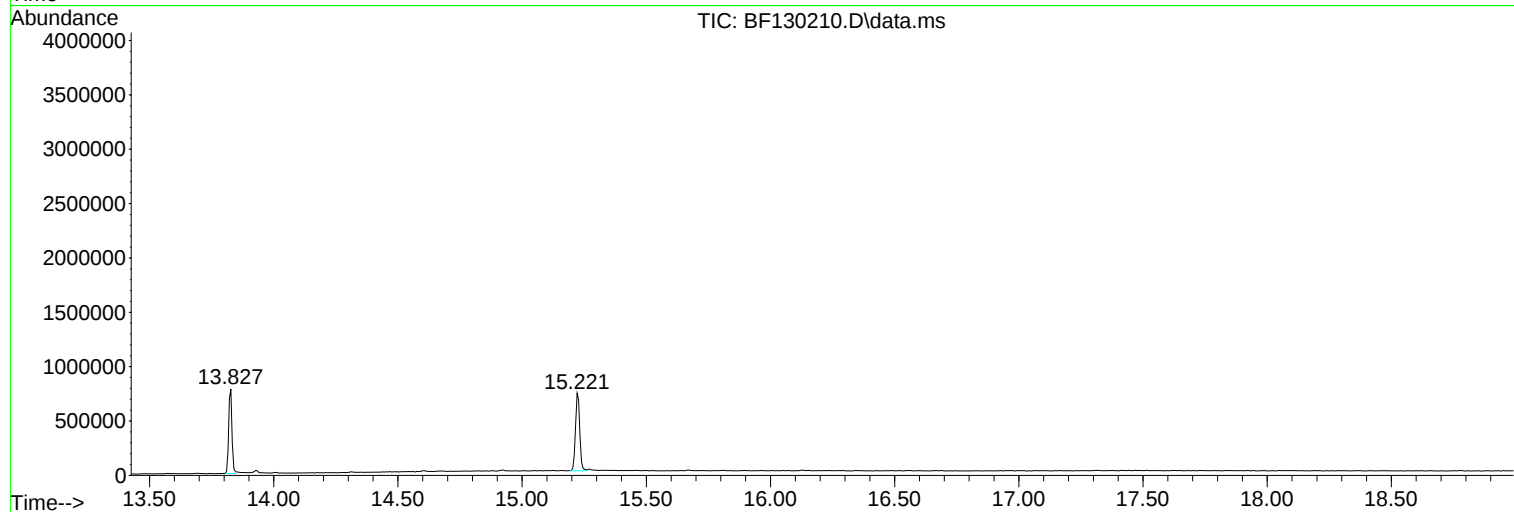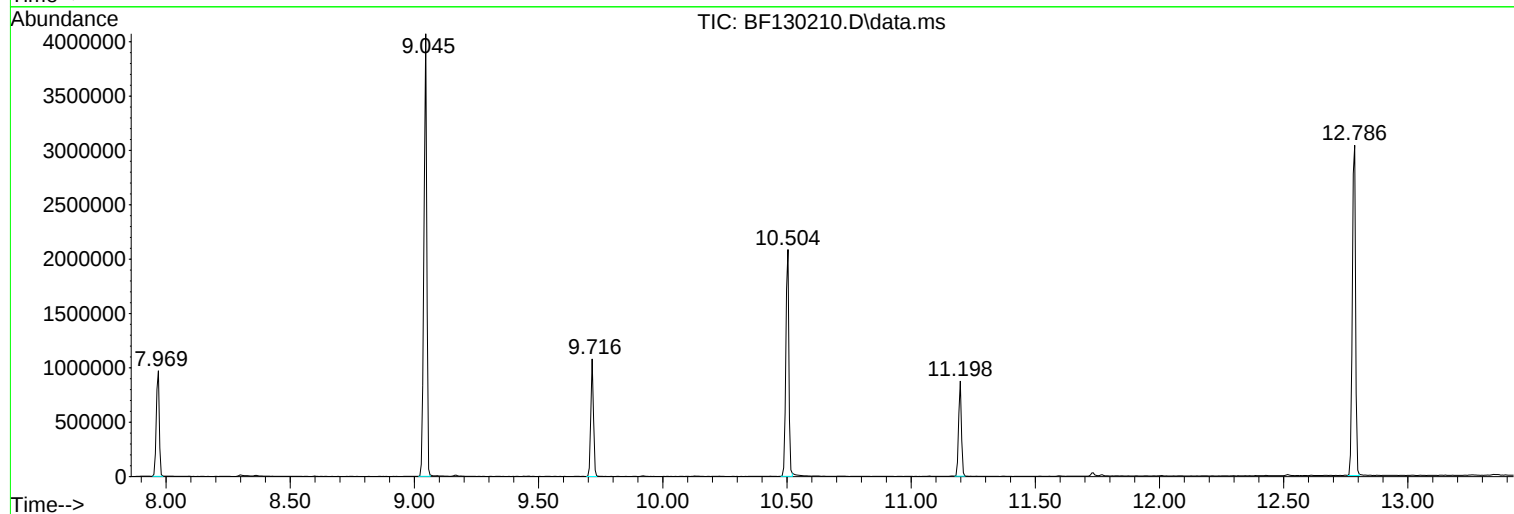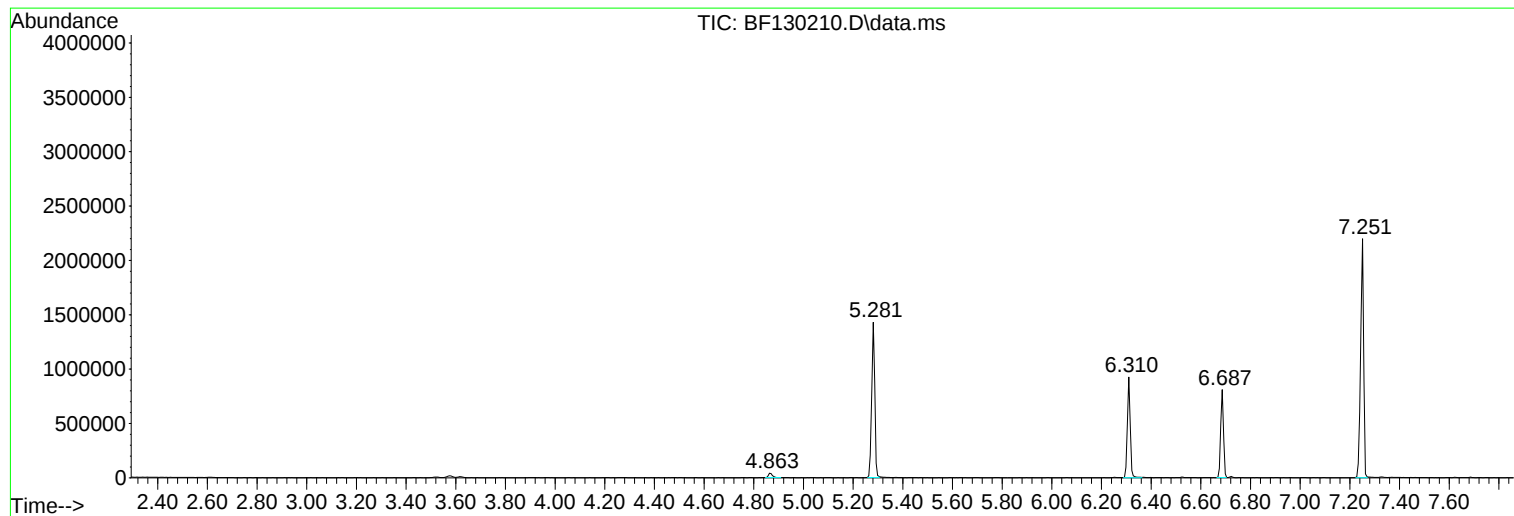

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
Data File : BF130210.D
Acq On : 12 Sep 2022 17:57
Operator : CG\JU
Sample : N4551-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
251032-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
Data File : BF130210.D
Acq On : 12 Sep 2022 17:57
Operator : CG\JU
Sample : N4551-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
251032-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------