

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
 Data File : BF130211.D
 Acq On : 12 Sep 2022 18:30
 Operator : CG\JU
 Sample : N4553-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 256074-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130211.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.869	436	439	448	rVB	71837	78122	1.73%	0.365%
2	5.287	505	510	513	rBV	2394344	2326847	51.43%	10.879%
3	6.310	680	684	702	rBV	1851254	1728862	38.21%	8.083%
4	6.686	744	748	751	rBV	1136506	848768	18.76%	3.968%
5	7.251	839	844	847	rBV	2372612	2151491	47.56%	10.059%
6	7.969	962	966	969	rBV	965930	850094	18.79%	3.975%
7	9.045	1144	1149	1152	rBV	5379709	4524160	100.00%	21.153%
8	9.716	1259	1263	1266	rBV	1430974	1096918	24.25%	5.129%
9	10.504	1392	1397	1400	rBV	2553179	2408148	53.23%	11.259%
10	11.192	1511	1514	1518	rBV	983164	868136	19.19%	4.059%
11	12.786	1780	1785	1788	rBV	3229035	3070977	67.88%	14.358%
12	13.827	1958	1962	1968	rBV	669398	662718	14.65%	3.099%
13	15.221	2194	2199	2205	rBV	677511	772858	17.08%	3.613%




Sum of corrected areas: 21388099

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
Data File : BF130211.D
Acq On : 12 Sep 2022 18:30
Operator : CG\JU
Sample : N4553-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
256074-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

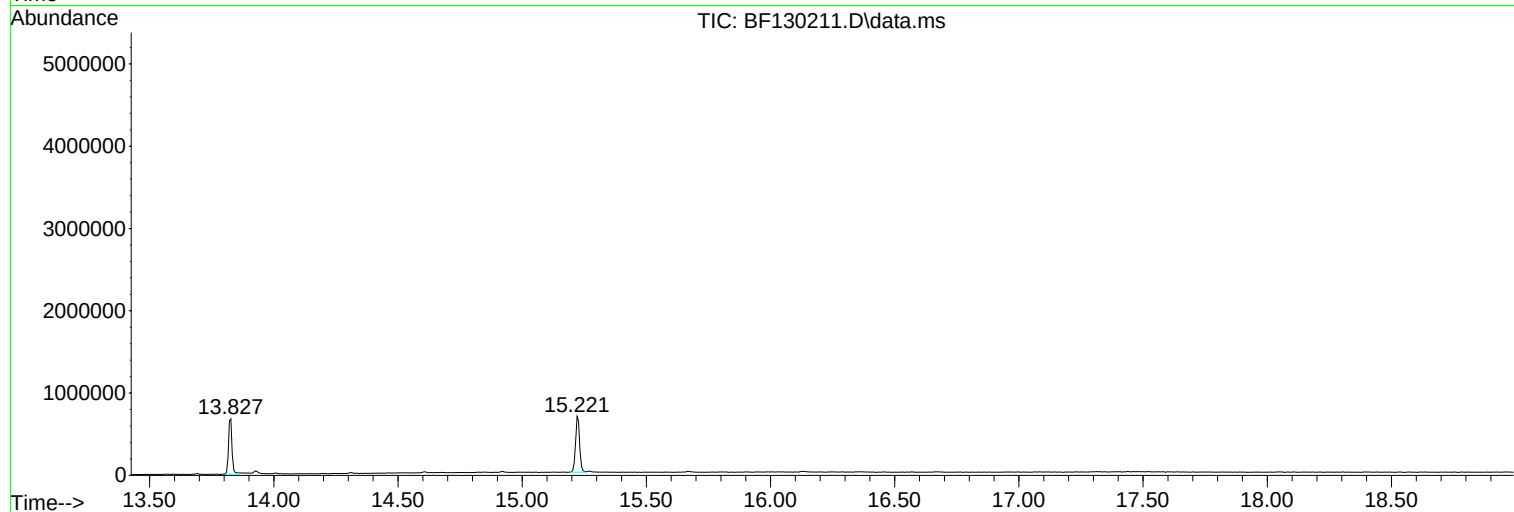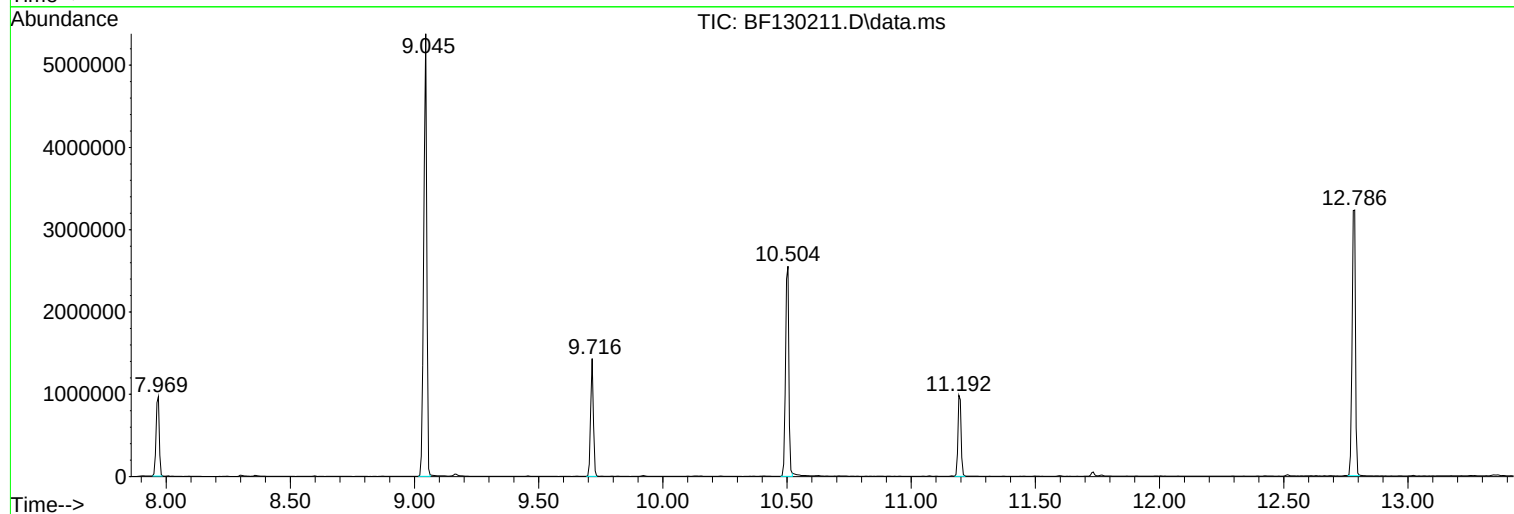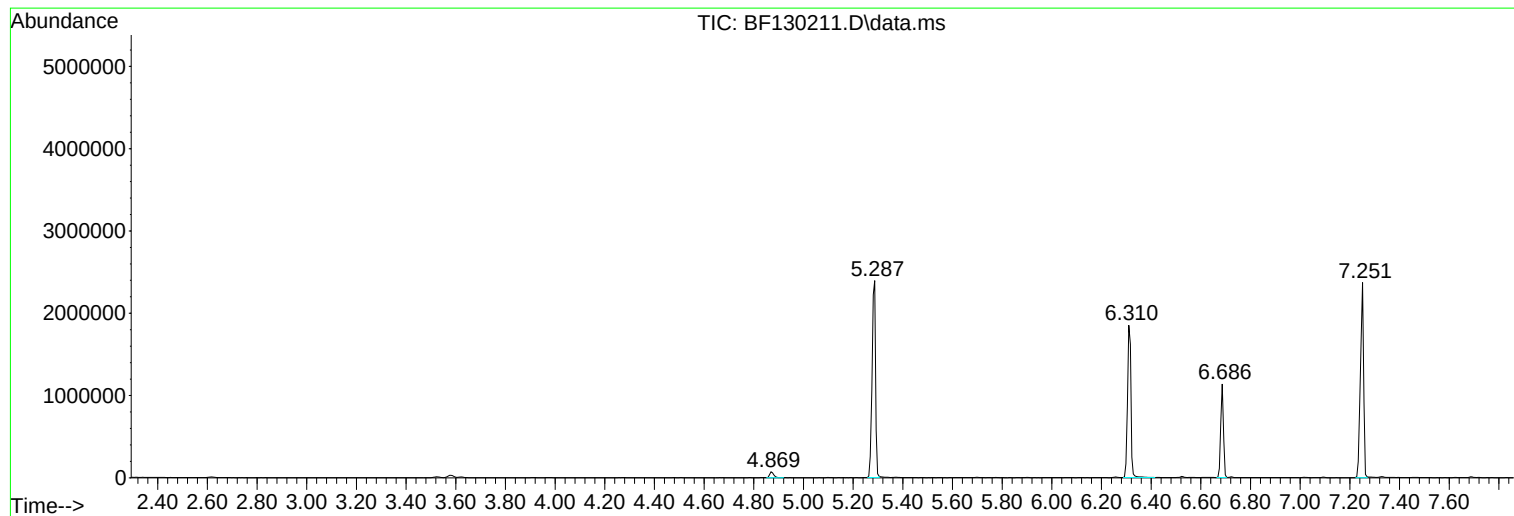

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
Data File : BF130211.D
Acq On : 12 Sep 2022 18:30
Operator : CG\JU
Sample : N4553-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
256074-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
Data File : BF130211.D
Acq On : 12 Sep 2022 18:30
Operator : CG\JU
Sample : N4553-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
256074-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------