

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
 Data File : BF130212.D
 Acq On : 12 Sep 2022 19:03
 Operator : CG\JU
 Sample : N4553-02
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 256074-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130212.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.587	216	221	225	rBV	35366	56284	1.68%	0.293%
2	3.628	225	228	234	rVB	29900	42804	1.27%	0.223%
3	4.869	436	439	447	rVB	127435	161554	4.81%	0.842%
4	5.287	505	510	513	rBV	2208164	2010056	59.84%	10.470%
5	6.310	680	684	688	rBV	1548742	1471823	43.82%	7.666%
6	6.687	744	748	751	rBV	890041	691214	20.58%	3.600%
7	7.251	839	844	847	rBV	2177447	1869453	55.66%	9.738%
8	7.963	961	965	969	rBV	1050497	918117	27.33%	4.782%
9	9.045	1144	1149	1152	rBV	4131453	3358961	100.00%	17.496%
10	9.716	1259	1263	1266	rBV	1261028	964931	28.73%	5.026%
11	10.498	1392	1396	1400	rBV	2088852	1923399	57.26%	10.019%
12	11.192	1511	1514	1518	rBV	947539	856931	25.51%	4.464%
13	12.780	1780	1784	1788	rBV	3595583	3257350	96.97%	16.967%
14	13.822	1958	1961	1968	rBV	796167	774448	23.06%	4.034%
15	15.221	2194	2199	2205	rBV	737255	840858	25.03%	4.380%




Sum of corrected areas: 19198183

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
Data File : BF130212.D
Acq On : 12 Sep 2022 19:03
Operator : CG\JU
Sample : N4553-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
256074-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

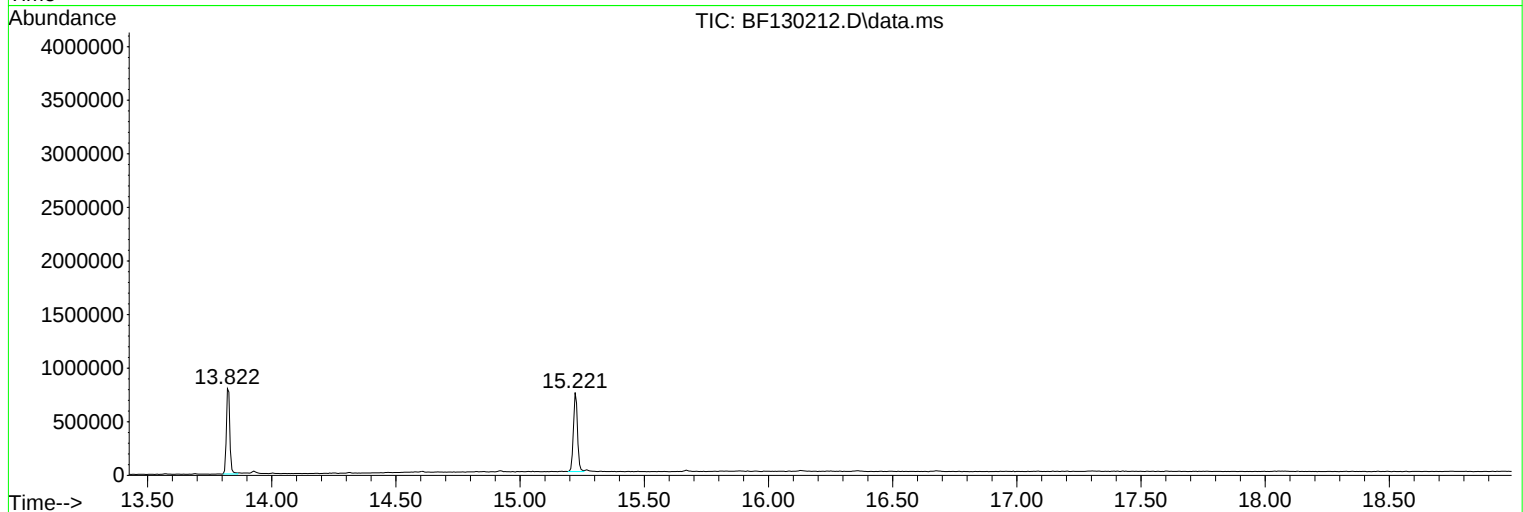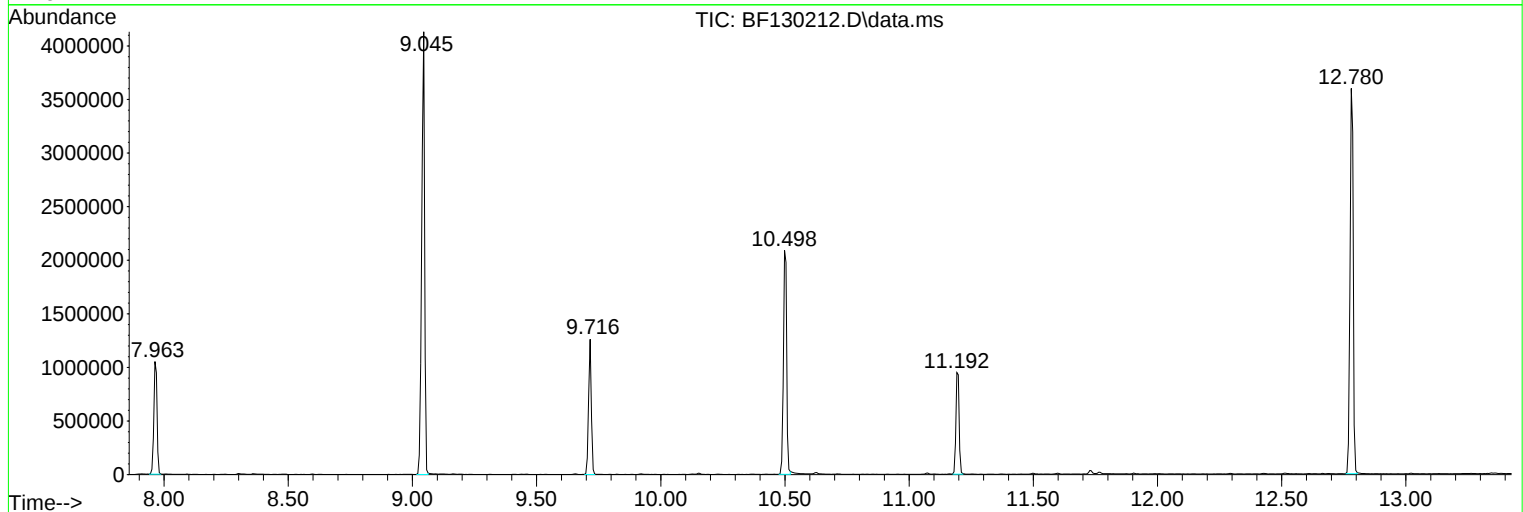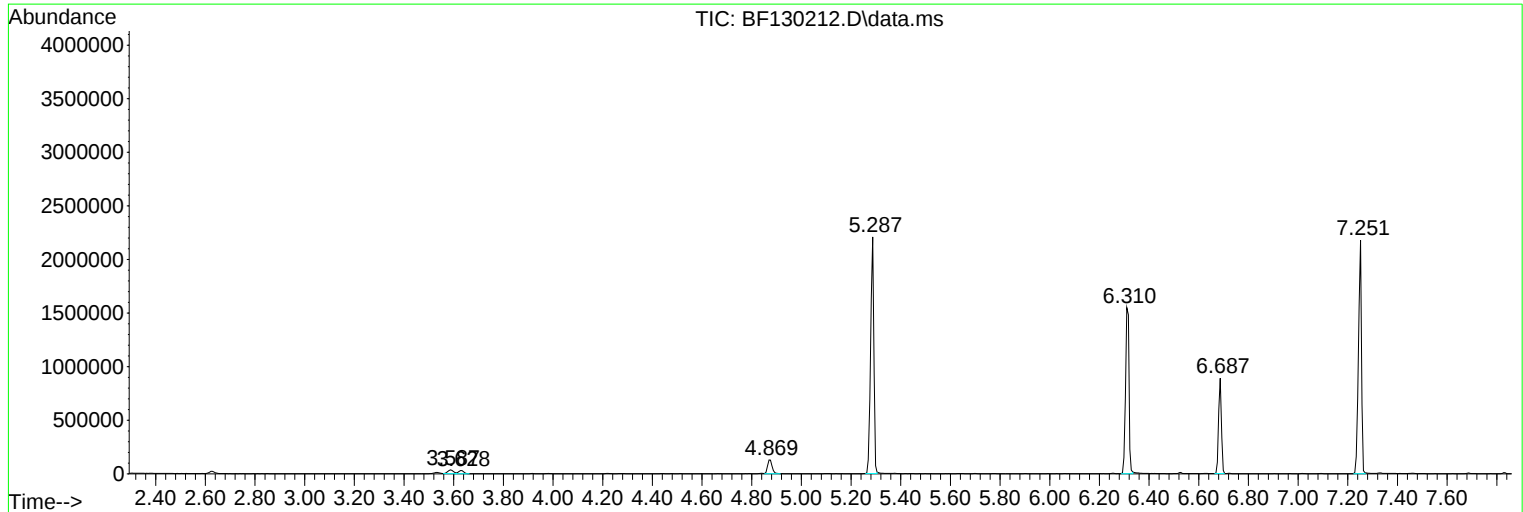

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
Data File : BF130212.D
Acq On : 12 Sep 2022 19:03
Operator : CG\JU
Sample : N4553-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
256074-2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.869	4.67 ng	161554	1,4-Dichlorobenzene-d4	6.687

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	27		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	12		
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9		

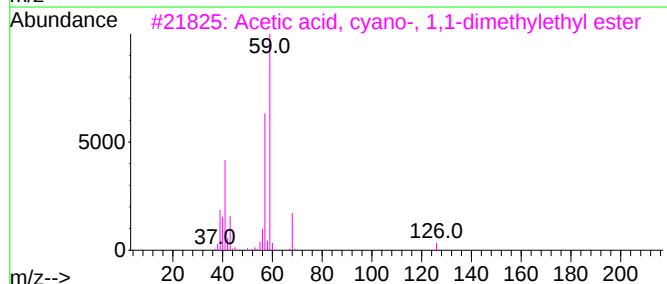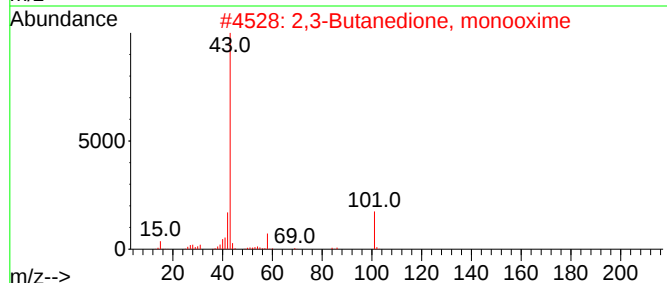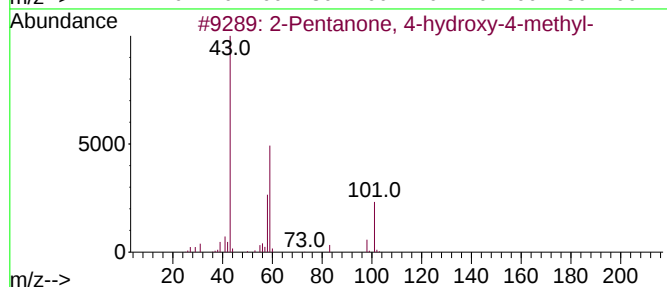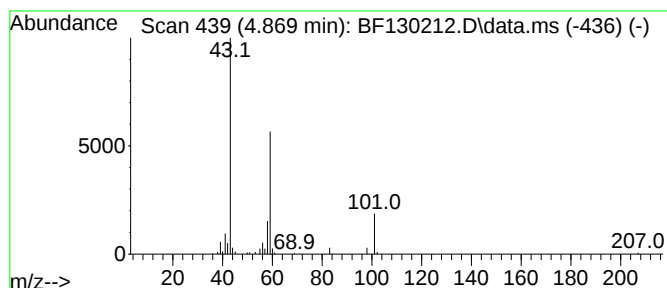

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
Data File : BF130212.D
Acq On : 12 Sep 2022 19:03
Operator : CG\JU
Sample : N4553-02
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
256074-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.869	4.7	ng	161554	1	6.687	691214	20.0