


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
 Data File : BF130204.D
 Acq On : 12 Sep 2022 10:52
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 07 02:05:07 2022

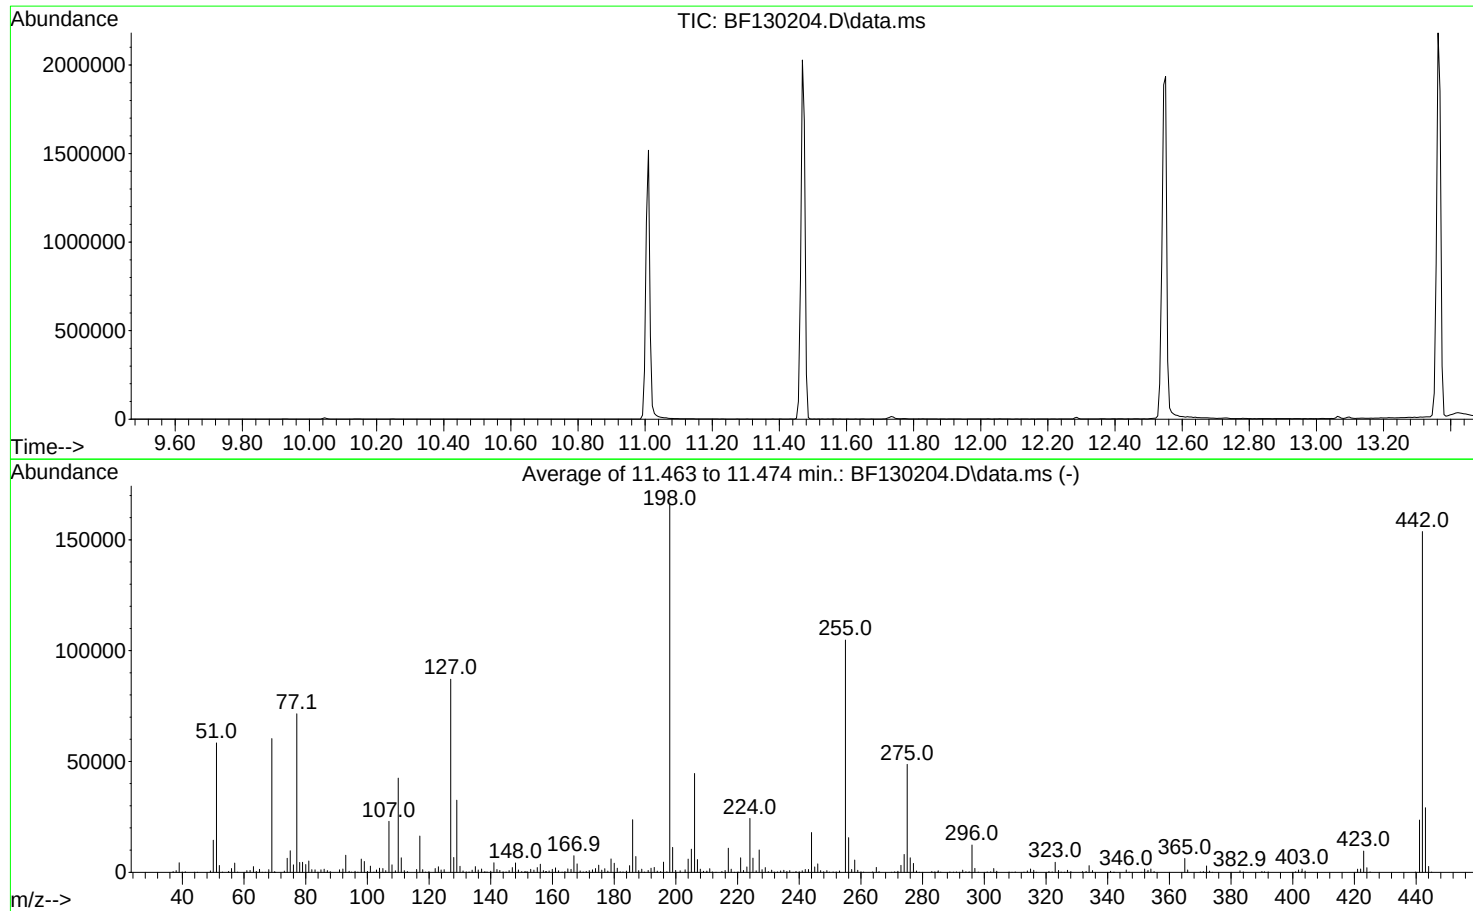




AutoFind: Scans 1560, 1561, 1562; Background Corrected with Scan 1555

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	58384	PASS
68	69	0.00	2	2.0	1194	PASS
69	198	0.00	100	36.4	60355	PASS
70	69	0.00	2	0.4	234	PASS
127	198	10	80	52.5	87128	PASS
197	198	0.00	2	0.2	267	PASS
198	198	100	100	100.0	165971	PASS
199	198	5	9	6.7	11198	PASS
275	198	10	60	29.4	48725	PASS
365	198	1	100	3.8	6235	PASS
441	198	0.01	100	14.2	23608	PASS
442	442	50	100	100.0	153757	PASS
443	442	15	24	19.0	29139	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
Data File : BF130204.D
Acq On : 12 Sep 2022 10:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 13 05:42:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 07 02:05:07 2022
Response via : Initial Calibration

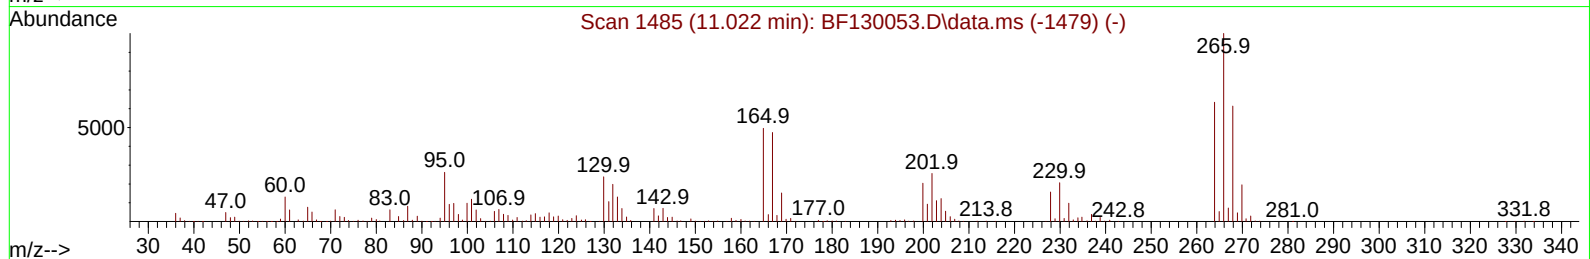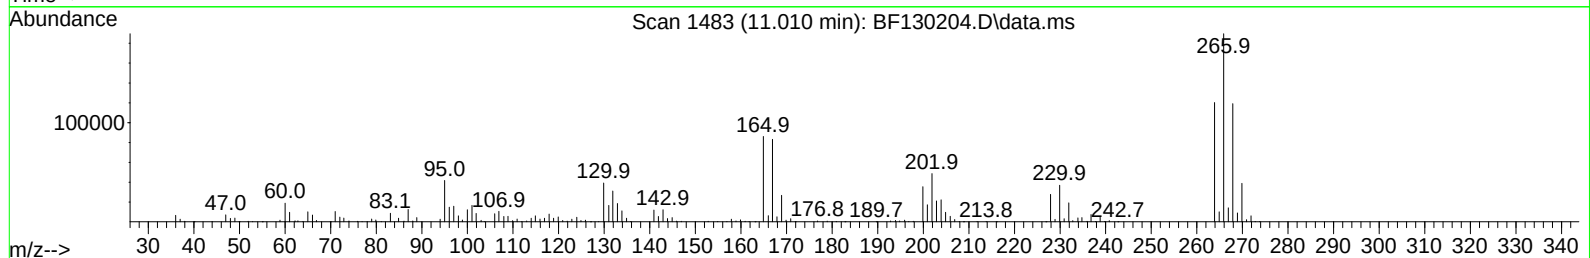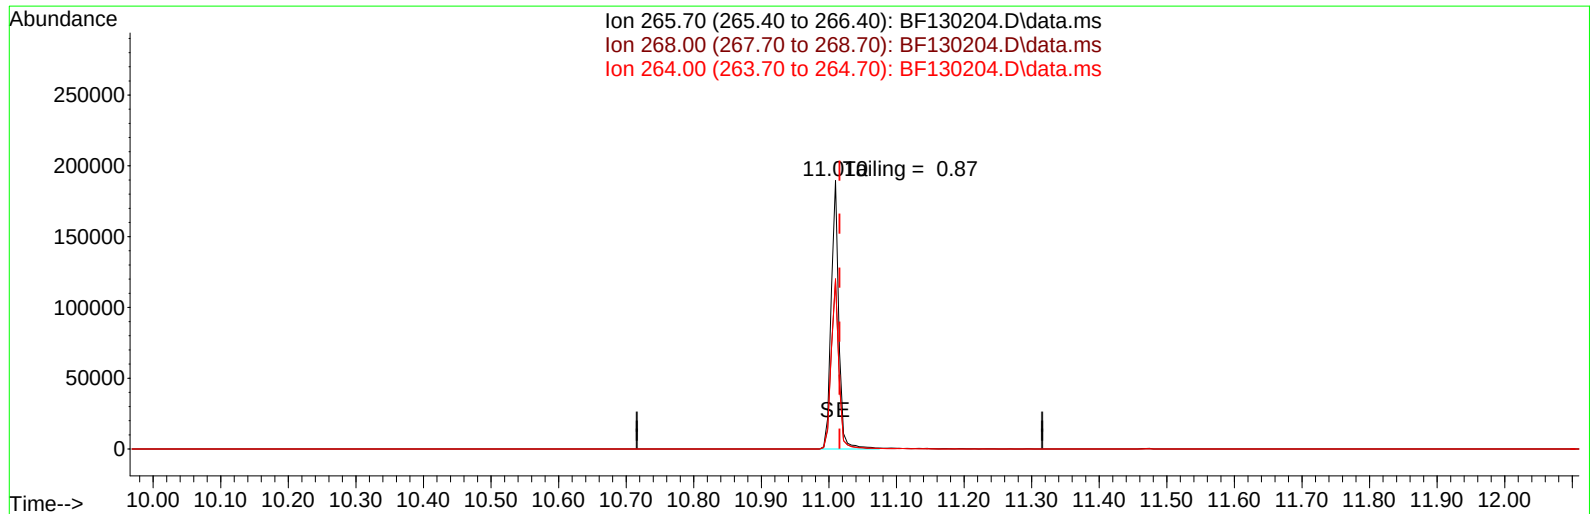

TIC: BF130204.D\data.ms

(70) Pentachlorophenol (C)

11.010min (-0.006) 26910.92 ng




response 150285

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.81
264.00	59.90	63.42
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091222\
Data File : BF130204.D
Acq On : 12 Sep 2022 10:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 13 05:42:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF083122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 07 02:05:07 2022
Response via : Initial Calibration

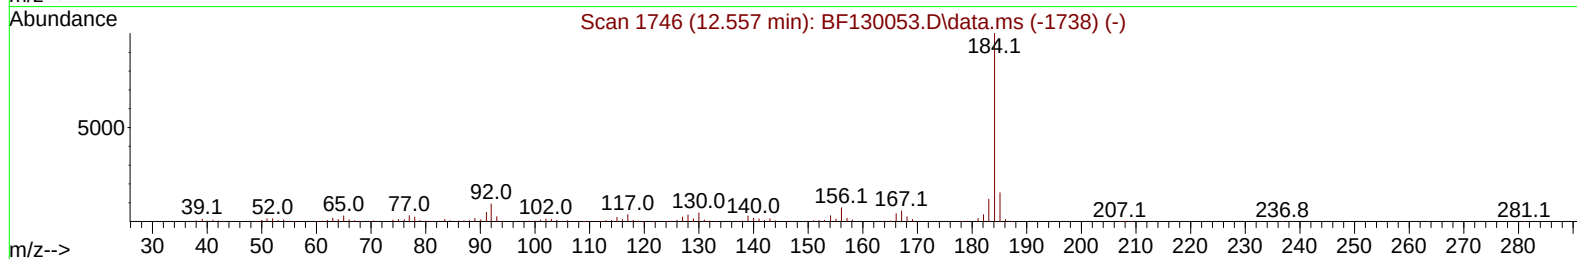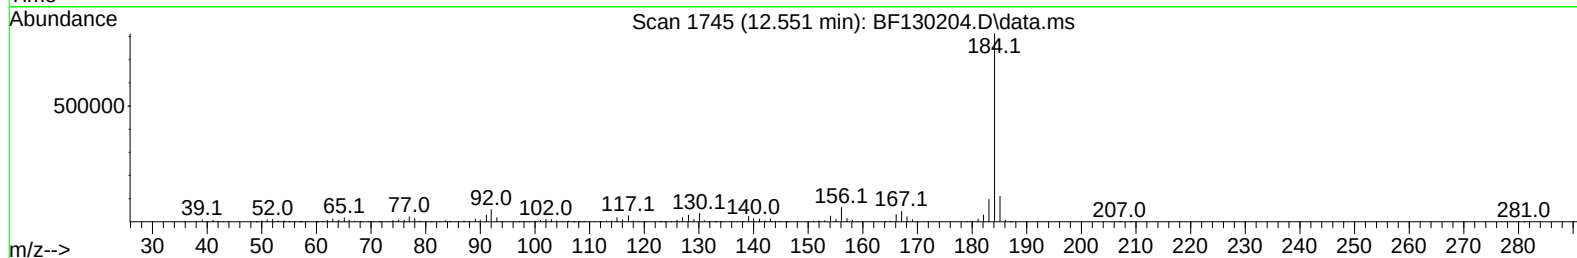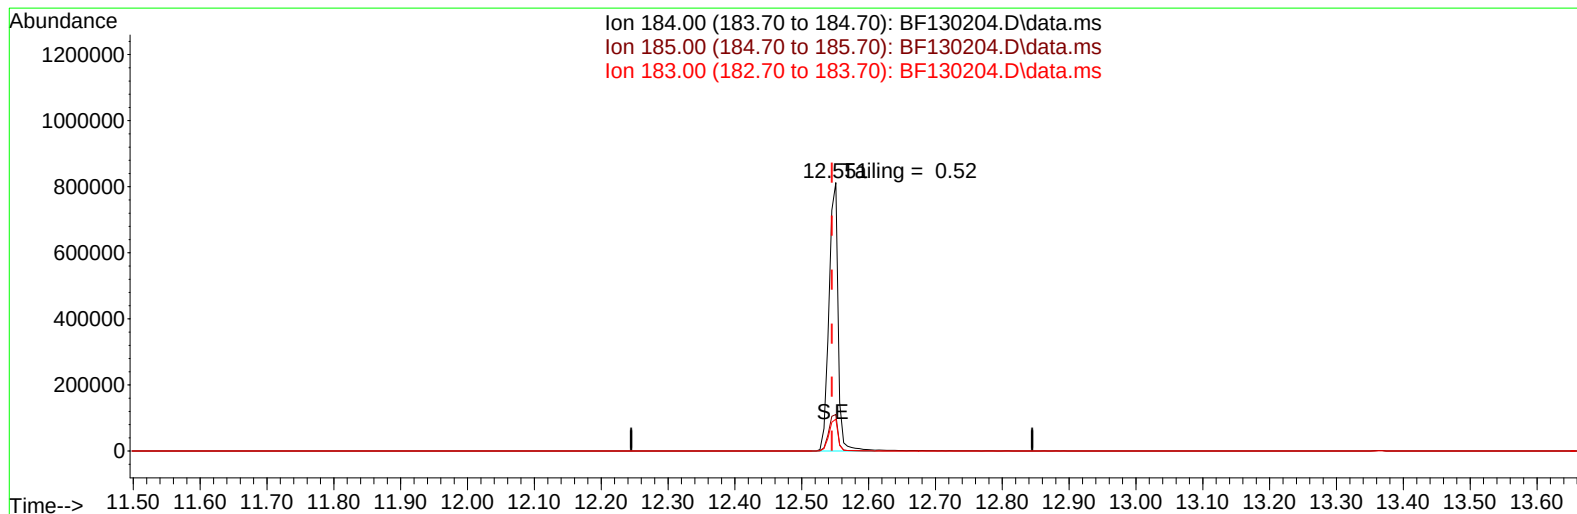

TIC: BF130204.D\data.ms

(77) Benzidine

12.551min (+ 0.006) 0.00 ng

response 774051

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.30	13.58
183.00	11.80	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/12/2022	BNA_F	BF130204.D
Compound Name	Response	Retention Time
DDT	350031	13.363
DDD	4026	13.063
DDE	608	12.733
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4634	354665	1.31

Instrument :
BNA_F
ClientSampleId :
DFTPP