
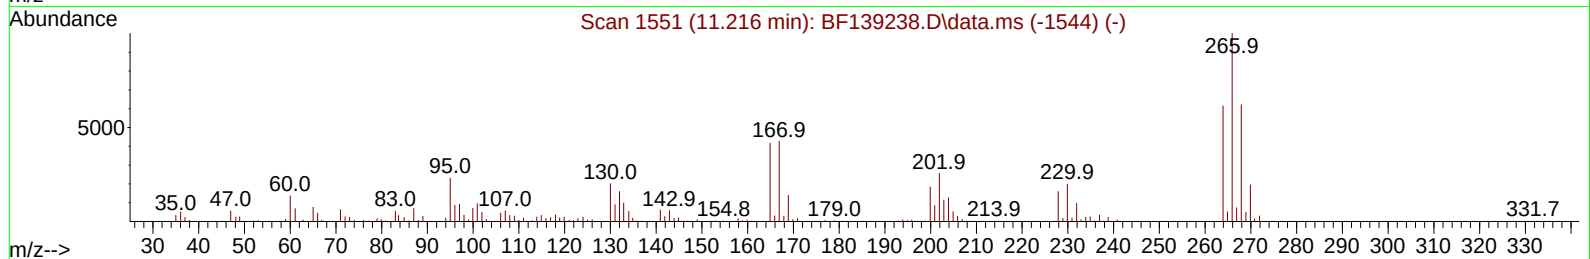
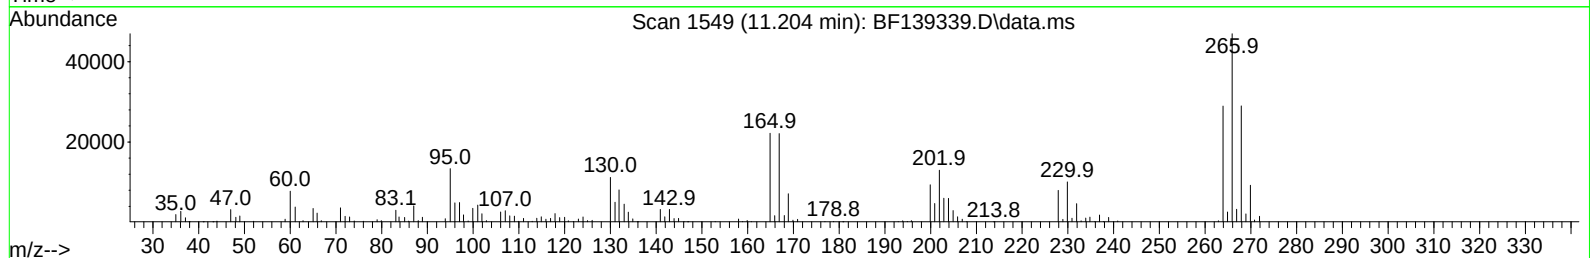


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091224\
Data File : BF139339.D
Acq On : 12 Sep 2024 11:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 12:04:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

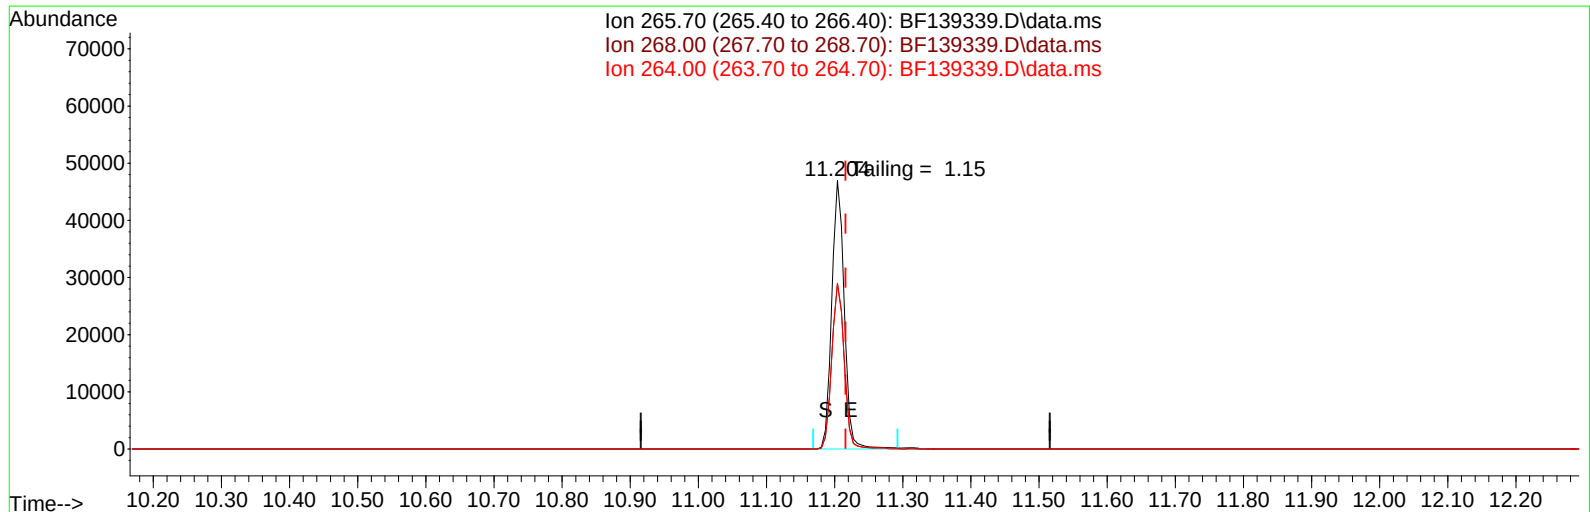

TIC: BF139339.D\data.ms




(70) Pentachlorophenol (C)

11.204min (-0.012) 35813.37 ng

response 59972

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	61.77
264.00	61.50	61.70
0.00	0.00	0.00

Quant Time: Sep 12 12:04:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

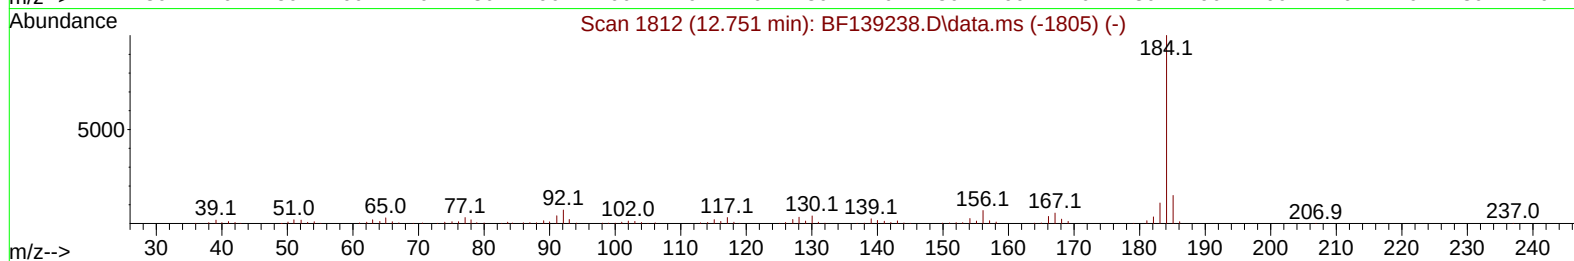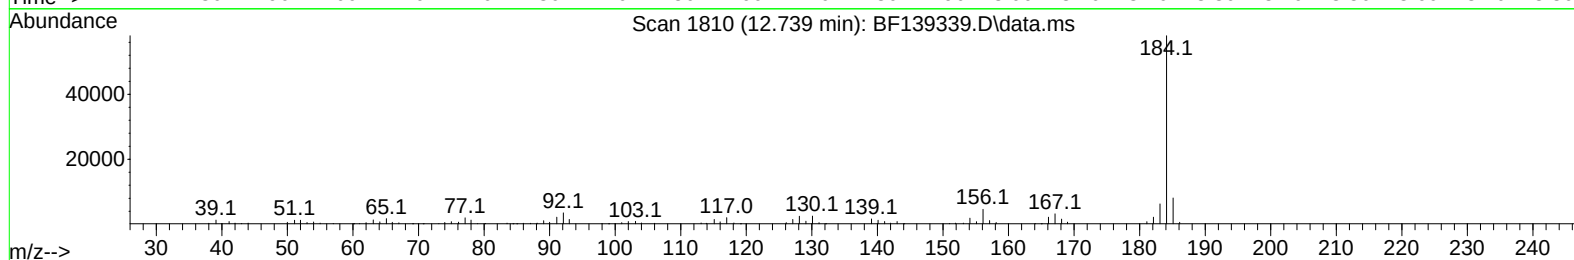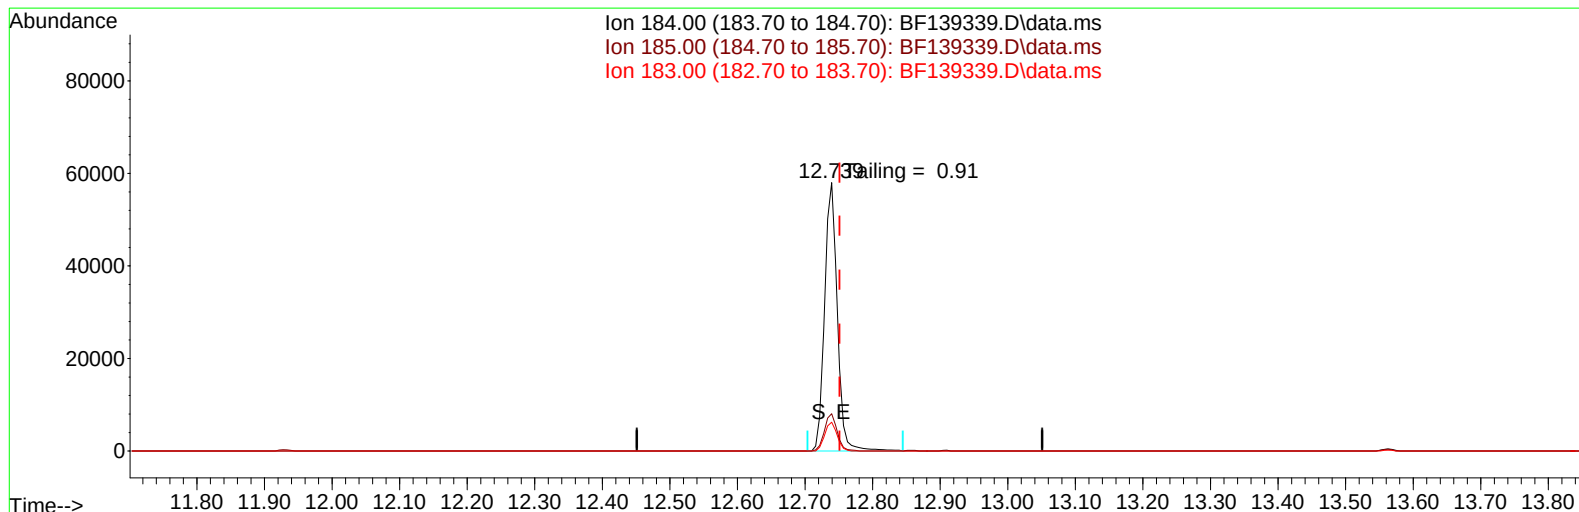

TIC: BF139339.D\data.ms

(77) Benzidine

12.739min (-0.012) 0.00 ng

response **75983**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.94
183.00	11.00	10.75
0.00	0.00	0.00