


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091224\
Data File : BF139339.D
Acq On : 12 Sep 2024 11:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 04 16:11:43 2024

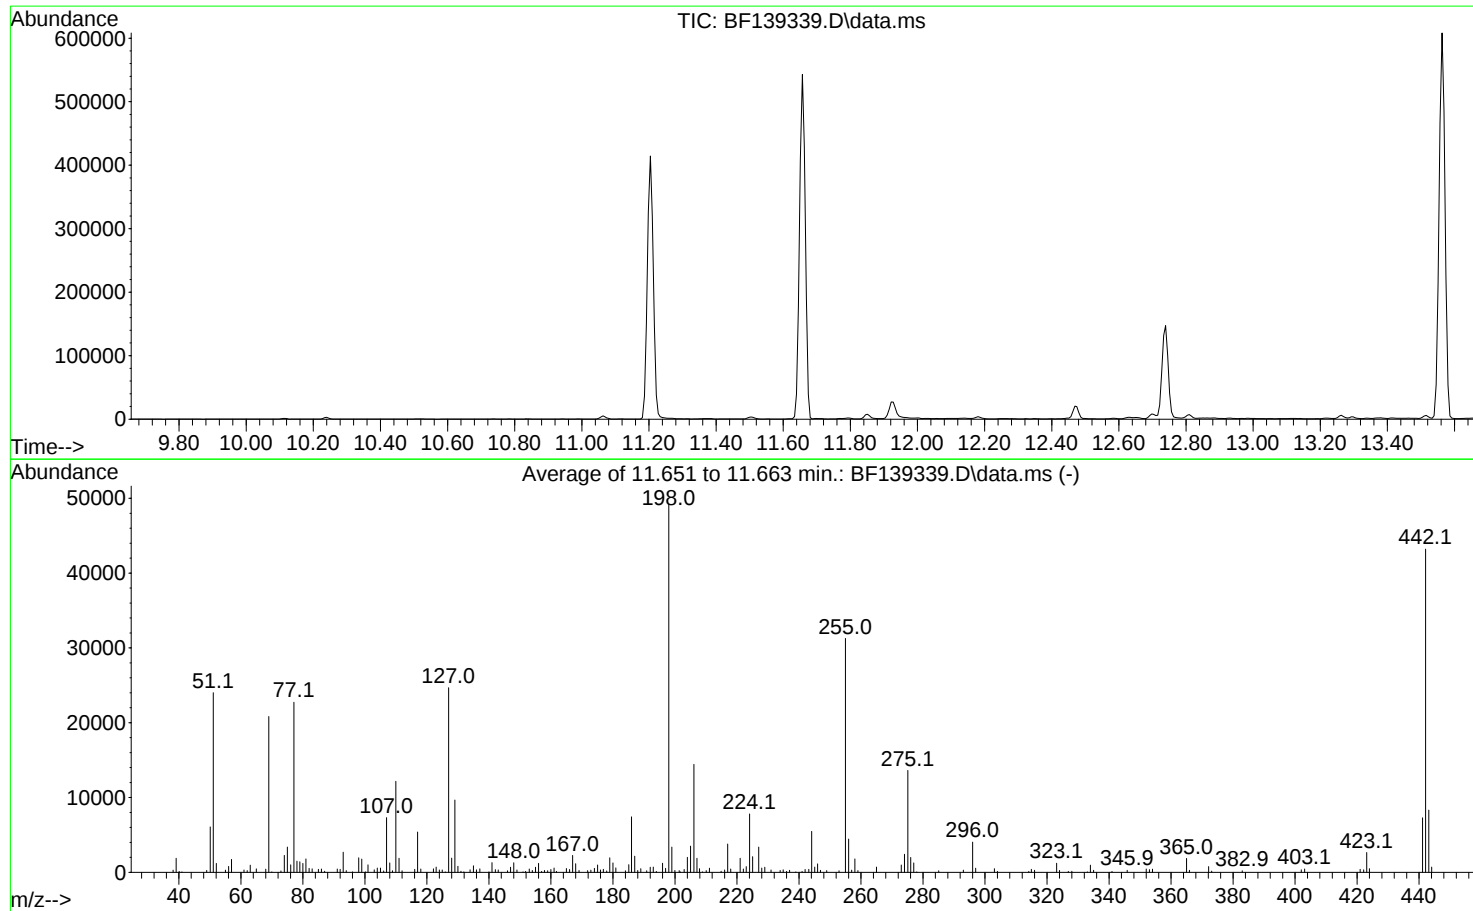


AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.8	24021	PASS
68	69	0.00	2	2.0	413	PASS
69	198	0.00	100	42.3	20819	PASS
70	69	0.00	2	0.2	50	PASS
127	198	10	80	50.2	24685	PASS
197	198	0.00	2	1.1	532	PASS
198	198	100	100	100.0	49184	PASS
199	198	5	9	6.8	3369	PASS
275	198	10	60	27.7	13617	PASS
365	198	1	100	3.8	1860	PASS
441	198	0.01	100	14.8	7286	PASS
442	442	50	100	100.0	43203	PASS
443	442	15	24	19.3	8321	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091224\
Data File : BF139339.D
Acq On : 12 Sep 2024 11:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 12 12:04:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

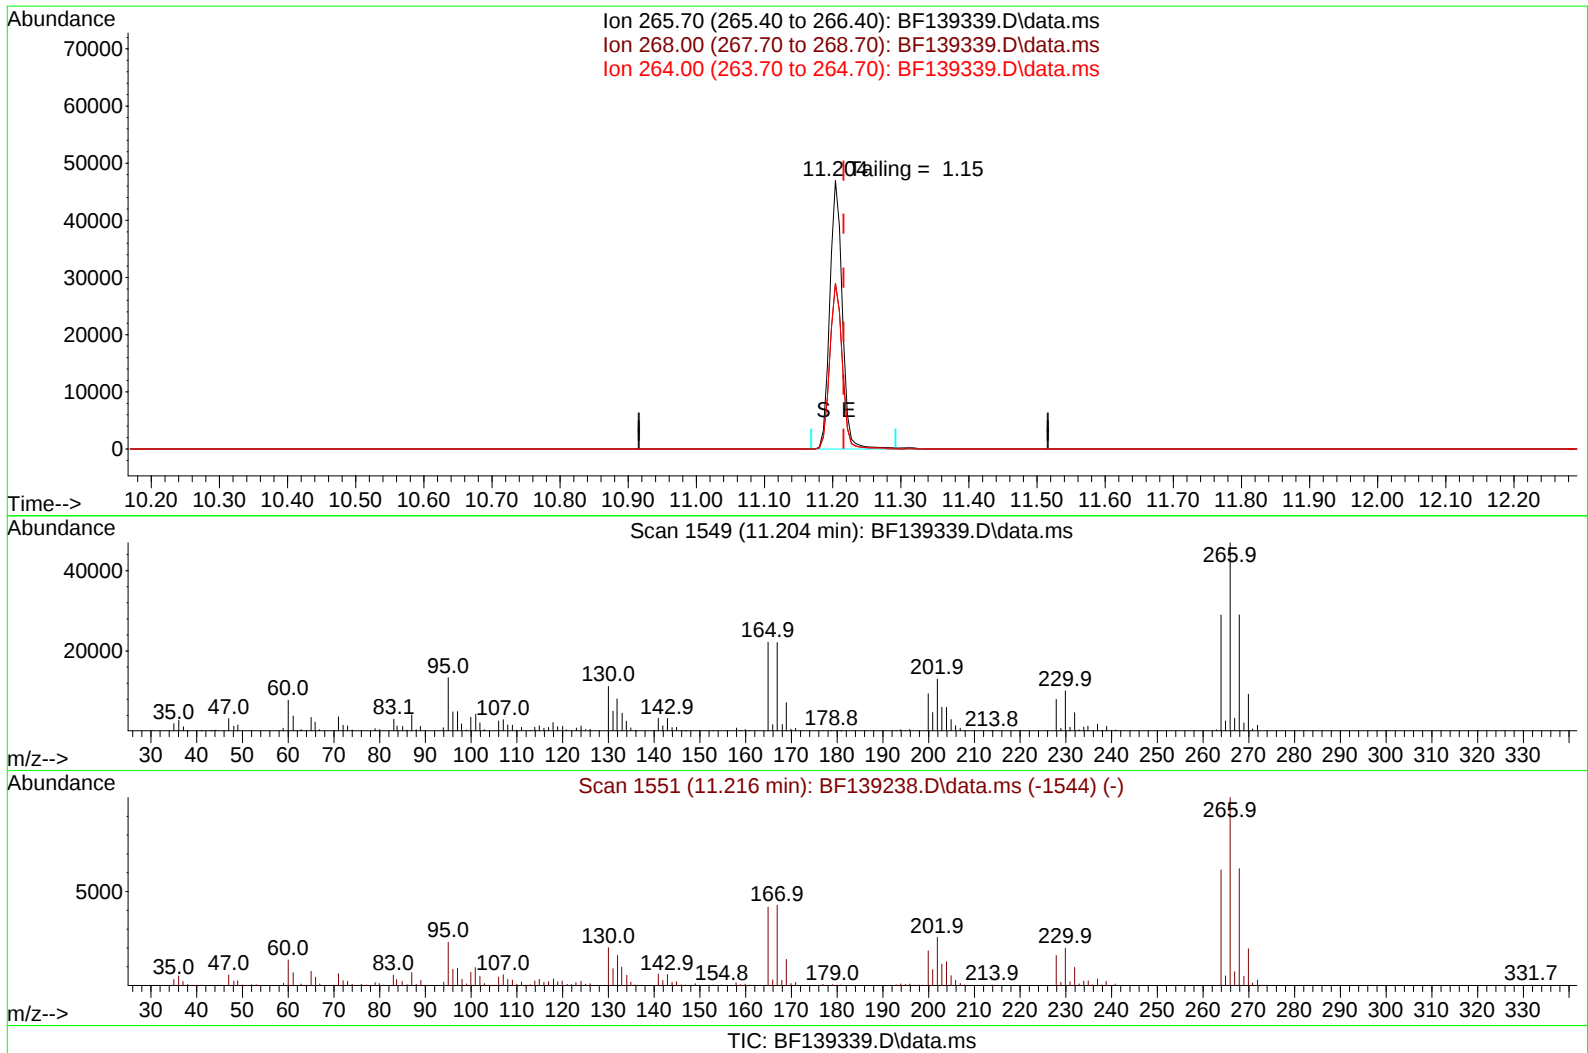

(70) Pentachlorophenol (C)

11.204min (-0.012) 35813.37 ng




response 59972

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.10	61.77
264.00	61.50	61.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091224\
Data File : BF139339.D
Acq On : 12 Sep 2024 11:19
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 12 12:04:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF090424.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 04 16:11:43 2024
Response via : Initial Calibration

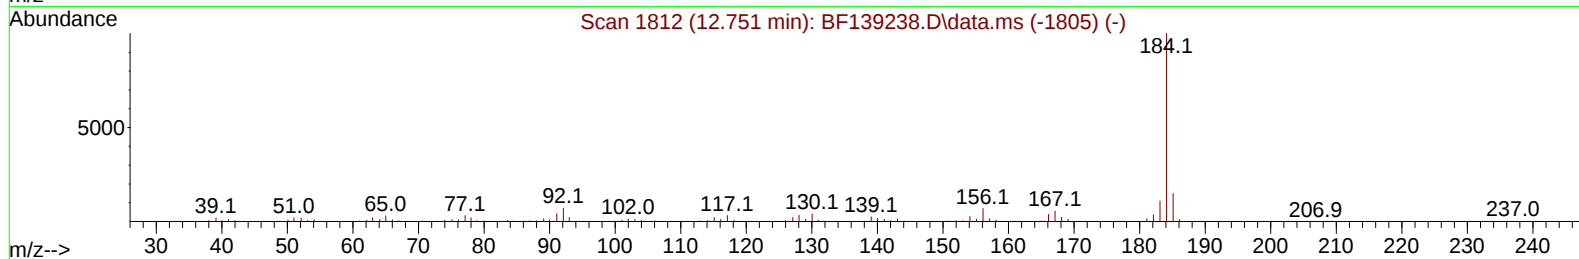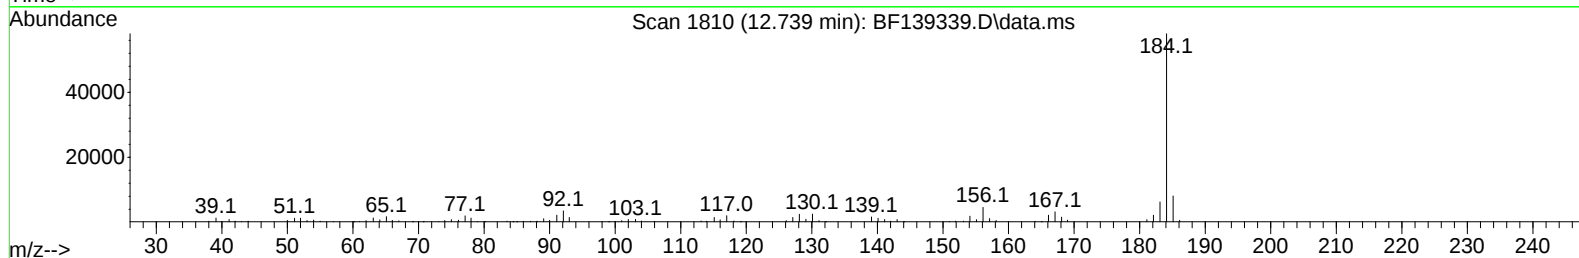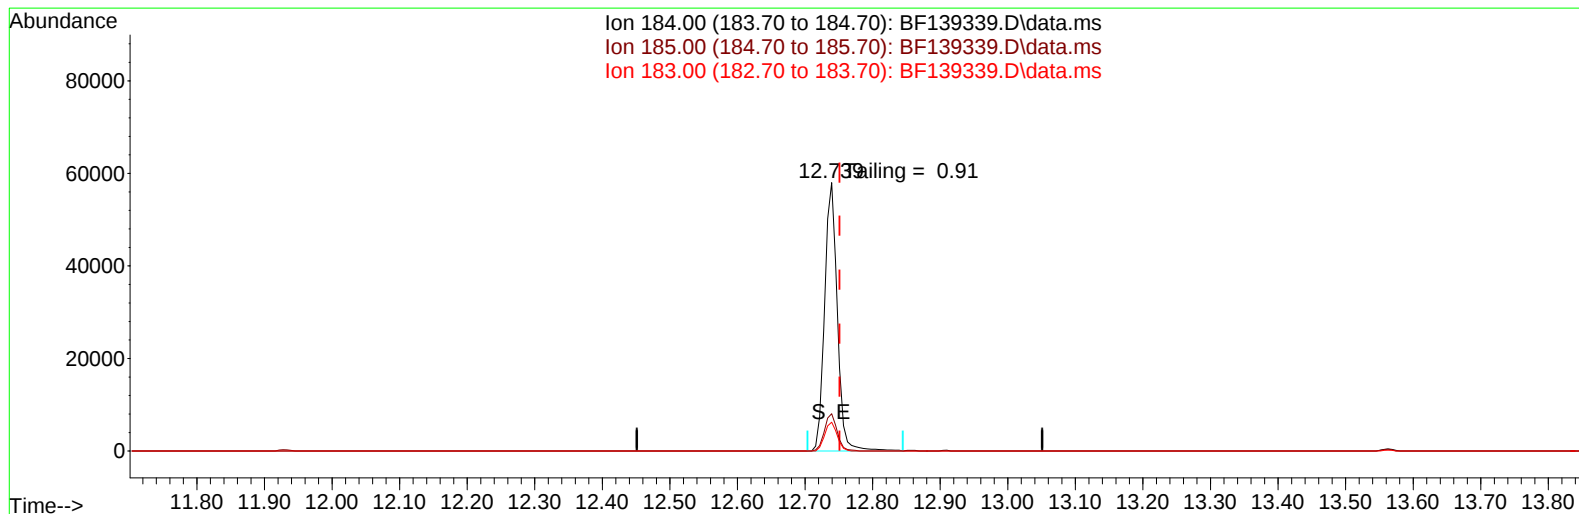

TIC: BF139339.D\data.ms

(77) Benzidine

12.739min (-0.012) 0.00 ng

response 75983

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	13.94
183.00	11.00	10.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/12/2024	BNA_F	<u>BF139339.D</u>
Compound Name	Response	Retention Time
DDT	141115	13.563
DDD	3332	13.263
DDE	301	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3633	144748	2.51

Instrument :
BNA_F
ClientSampleId :
DFTPP