
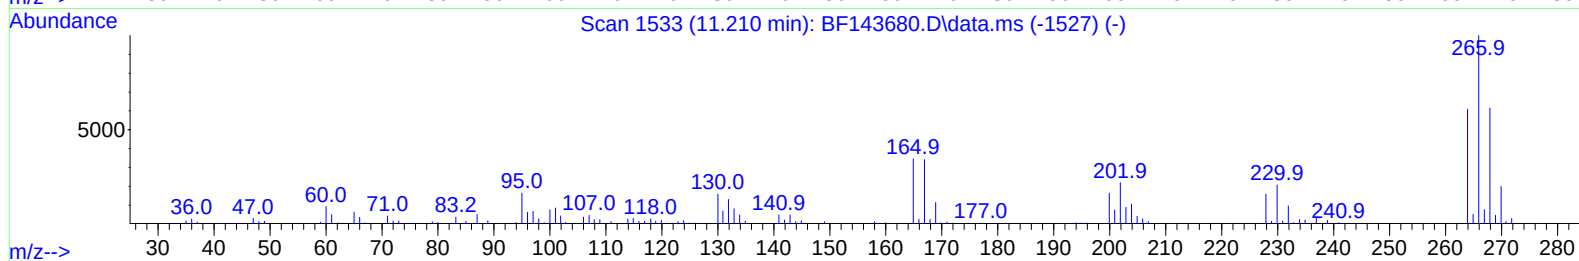
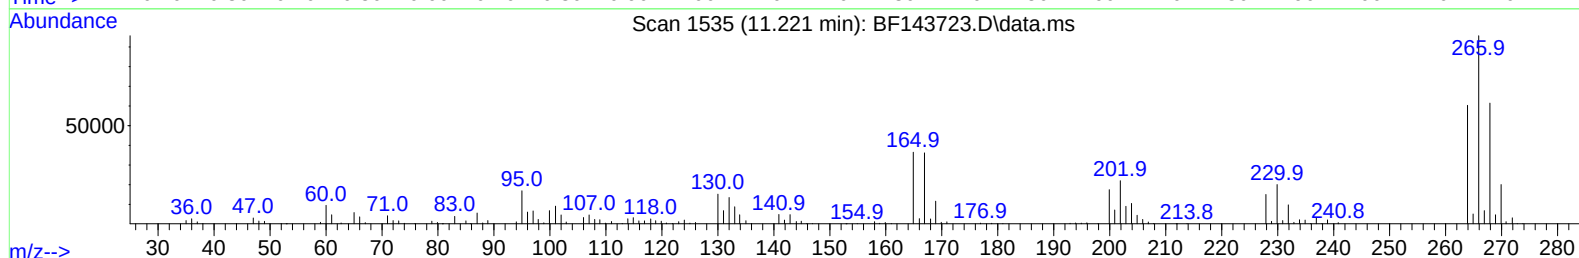


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091225\
Data File : BF143723.D
Acq On : 12 Sep 2025 10:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 10:45:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 15:20:16 2025
Response via : Initial Calibration

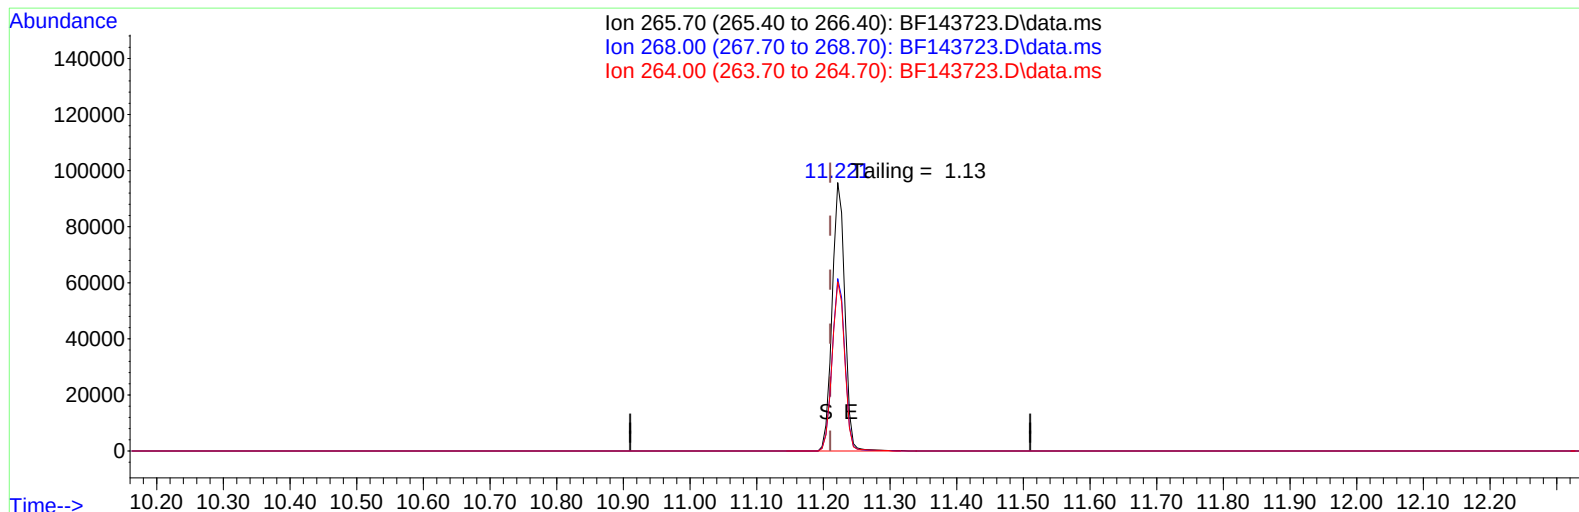

TIC: BF143723.D\data.ms

(70) Pentachlorophenol (C)




11.221min (+ 0.011) 36182.88 ng

response 126443

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	64.23
264.00	60.80	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091225\
Data File : BF143723.D
Acq On : 12 Sep 2025 10:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 12 10:45:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 15:20:16 2025
Response via : Initial Calibration

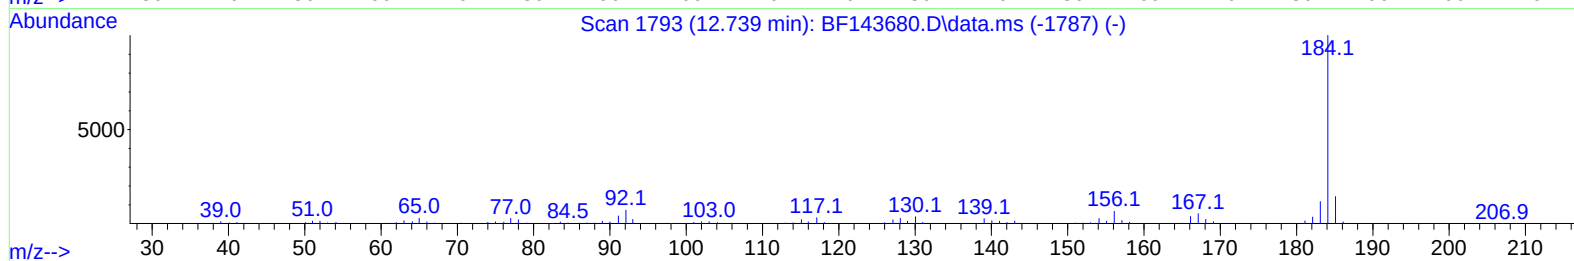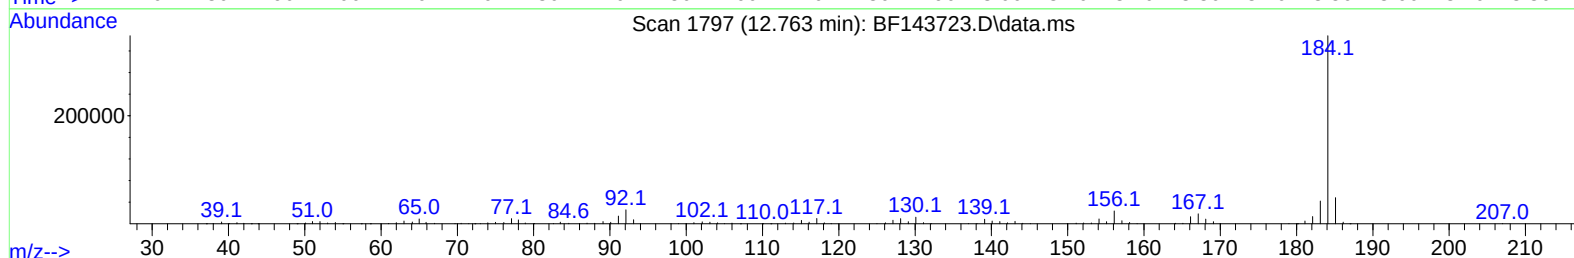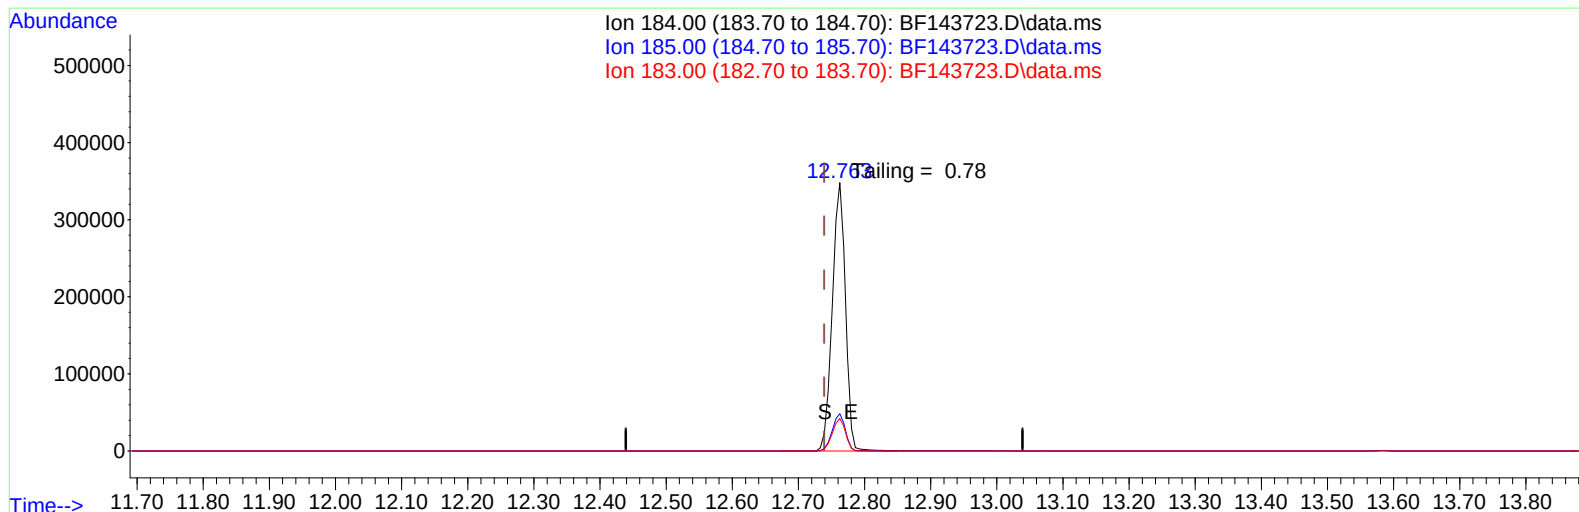

TIC: BF143723.D\data.ms

(77) Benzidine

12.763min (+ 0.023) 61529.69 ng

response 483562

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.92
183.00	11.80	12.11
0.00	0.00	0.00