

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091225\
 Data File : BF143737.D
 Acq On : 12 Sep 2025 17:09
 Operator : RC/JU
 Sample : Q3054-08
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MH-384

Quant Time: Sep 12 17:36:23 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 09 15:20:16 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.898	152	25651	20.000	ng	0.00
21) Naphthalene-d8	8.175	136	90191	20.000	ng	0.00
39) Acenaphthene-d10	9.933	164	42668	20.000	ng	0.00
64) Phenanthrene-d10	11.416	188	68736	20.000	ng	0.00
76) Chrysene-d12	14.057	240	73789	20.000	ng	0.01
86) Perylene-d12	15.545	264	71747	20.000	ng	0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.522	112	204078	135.740	ng	0.02
7) Phenol-d6	6.516	99	217371	118.743	ng	0.01
23) Nitrobenzene-d5	7.451	82	153504	105.865	ng	0.00
42) 2,4,6-Tribromophenol	10.722	330	63214	147.010	ng	0.01
45) 2-Fluorobiphenyl	9.251	172	318022	112.592	ng	0.00
79) Terphenyl-d14	13.010	244	355092	77.984	ng	0.02


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091225\
Data File : BF143737.D
Acq On : 12 Sep 2025 17:09
Operator : RC/JU
Sample : Q3054-08
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-384

Quant Time: Sep 12 17:36:23 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 15:20:16 2025
Response via : Initial Calibration




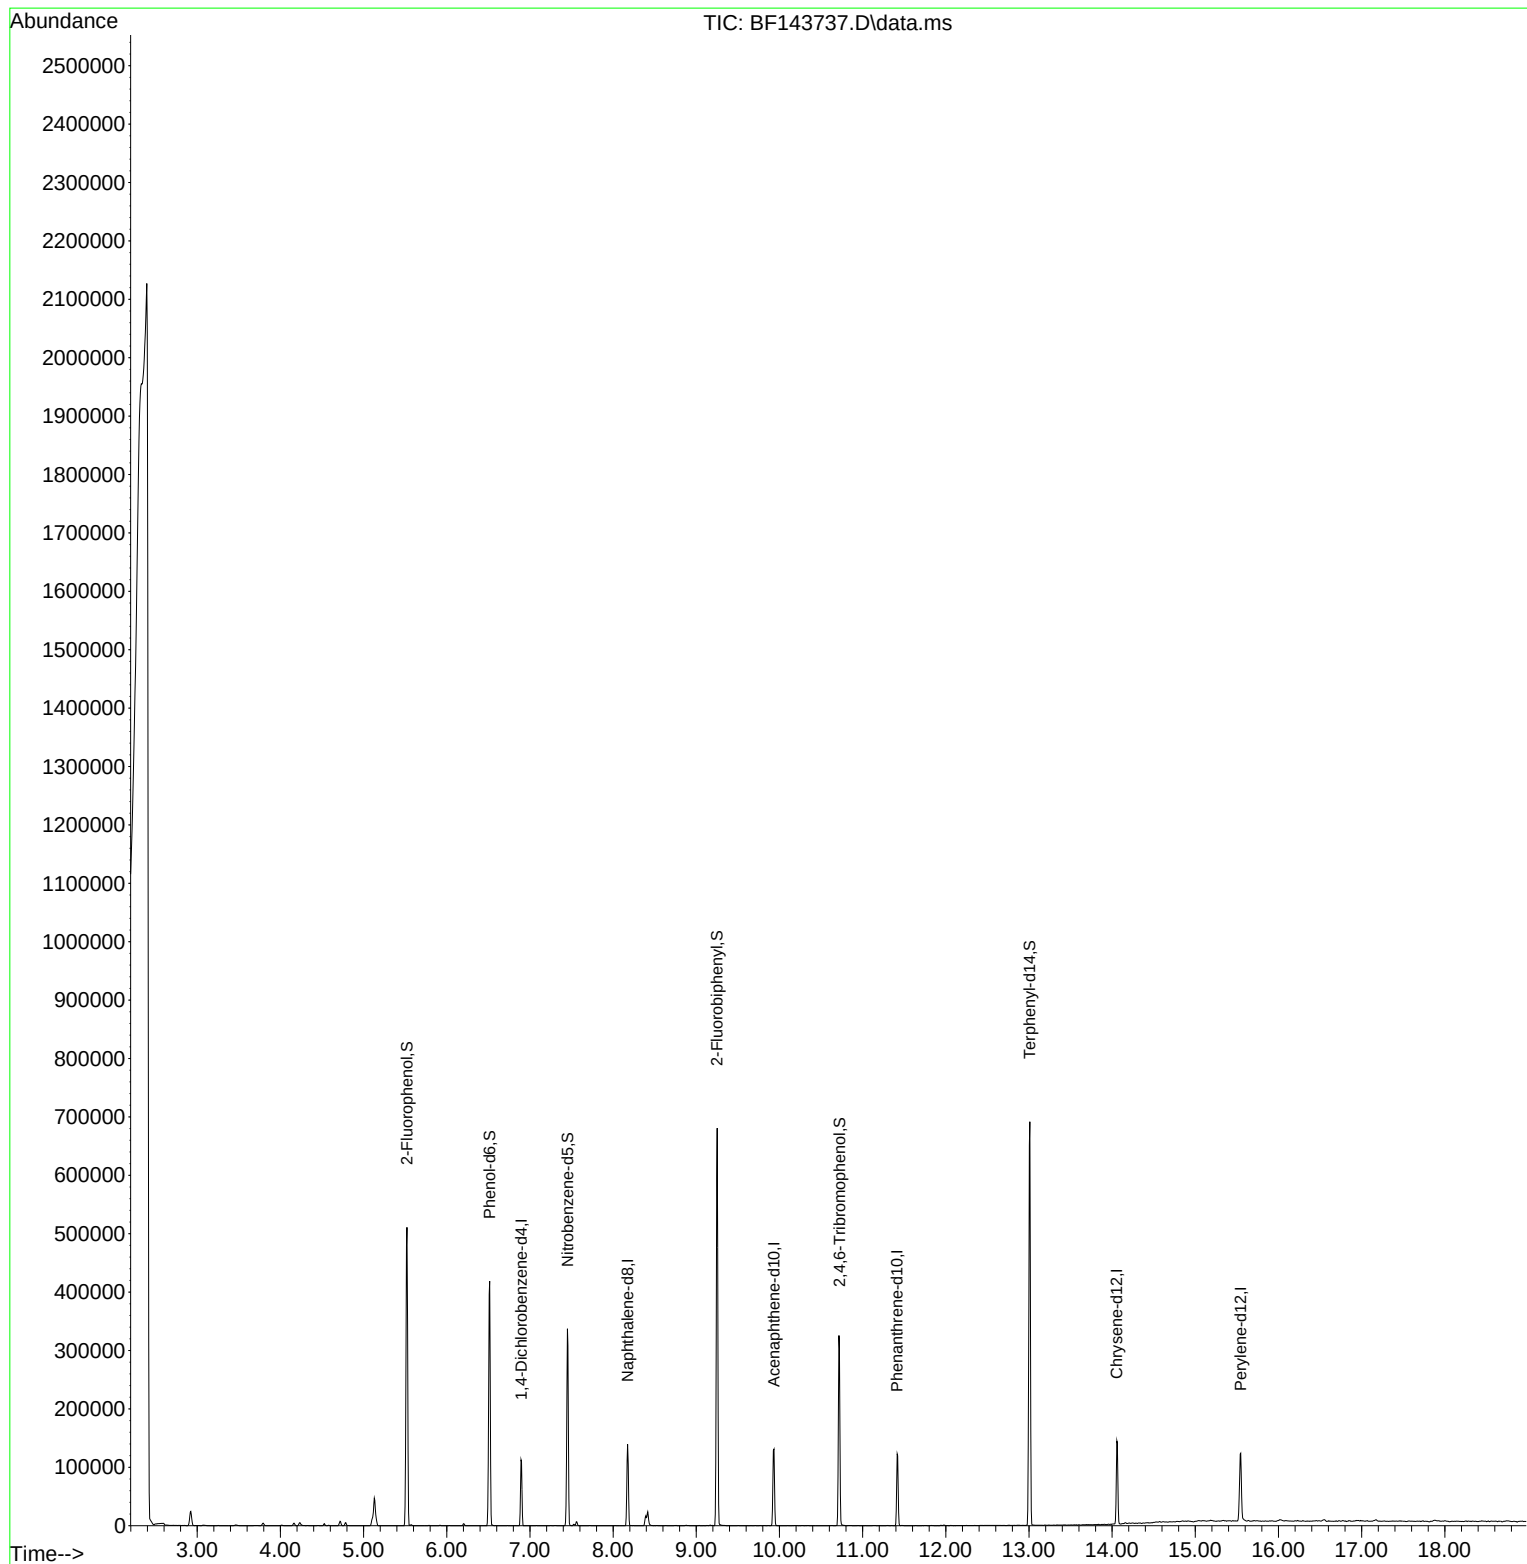


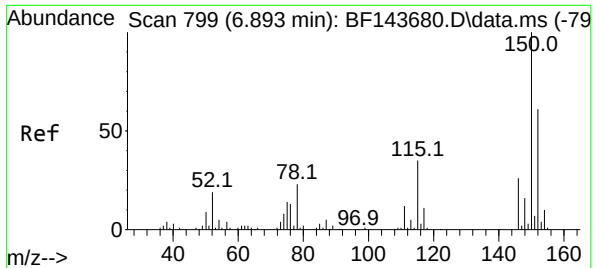

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.898 min Scan# 80
 Delta R.T. 0.005 min
 Lab File: BF143737.D
 Acq: 12 Sep 2025 17:09




Instrument :
 BNA_F
 ClientSampleId :
 MH-384


Tgt Ion:152 Resp: 25651
 Ion Ratio Lower Upper
 152 100
 150 158.7 130.7 196.1
 115 55.5 45.9 68.9

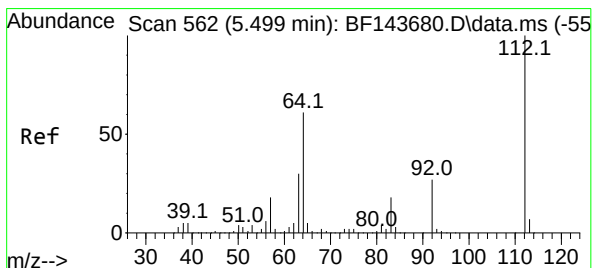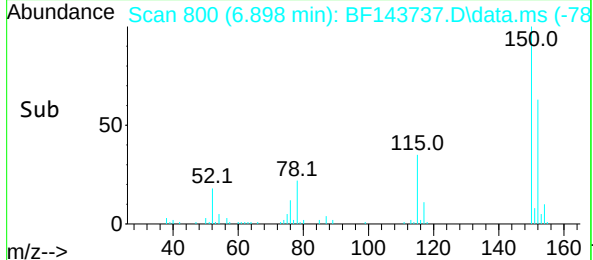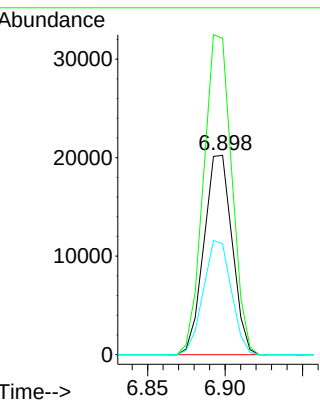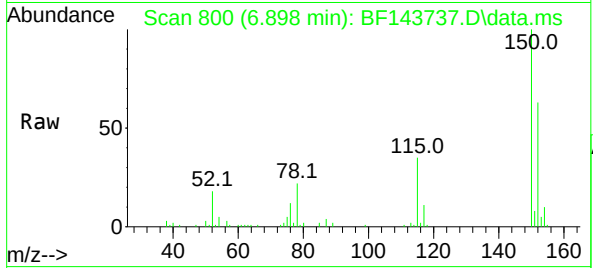

#5
 2-Fluorophenol
 Concen: 135.740 ng
 RT: 5.522 min Scan# 566
 Delta R.T. 0.023 min
 Lab File: BF143737.D
 Acq: 12 Sep 2025 17:09

Tgt Ion:112 Resp: 204078
 Ion Ratio Lower Upper
 112 100
 64 58.5 49.0 73.4
 63 29.5 24.3 36.5


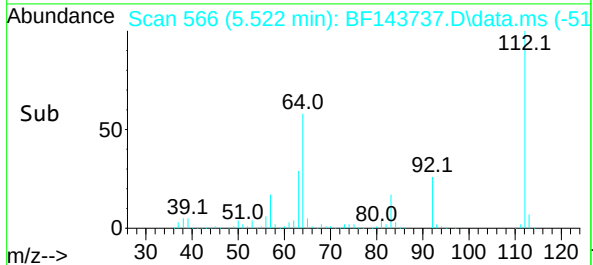
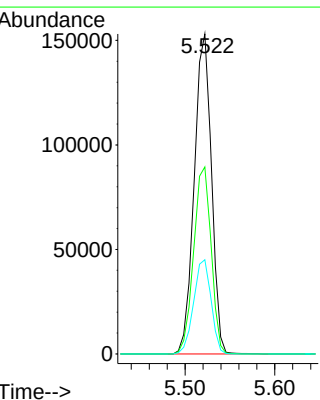
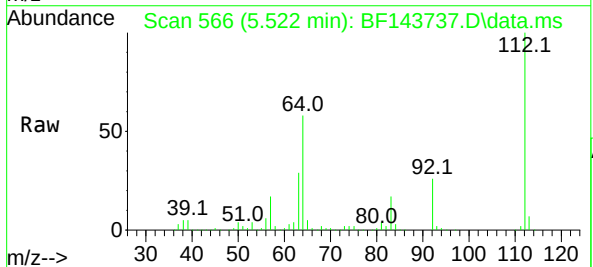


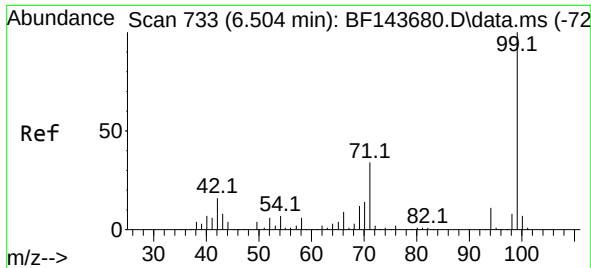

#7
Phenol-d6
Concen: 118.743 ng
RT: 6.516 min Scan# 71
Delta R.T. 0.012 min
Lab File: BF143737.D
Acq: 12 Sep 2025 17:09




Instrument :
BNA_F
ClientSampleId :
MH-384


Tgt Ion: 99 Resp: 217371
Ion Ratio Lower Upper
99 100
42 14.5 13.0 19.4
71 31.8 27.4 41.2

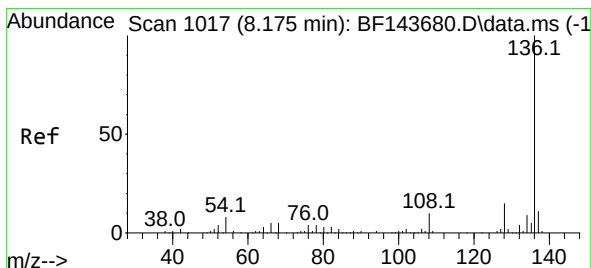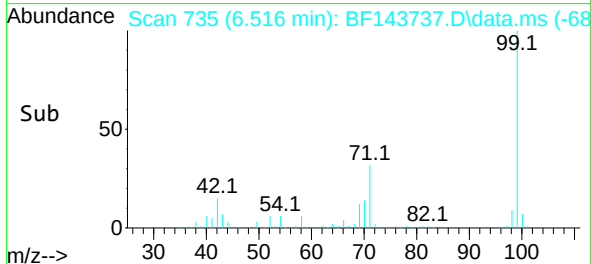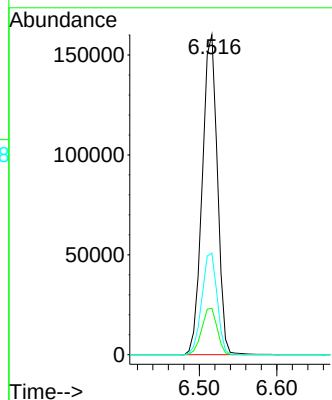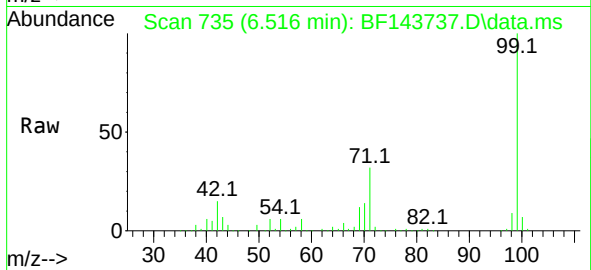

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.175 min Scan# 1017
Delta R.T. -0.000 min
Lab File: BF143737.D
Acq: 12 Sep 2025 17:09

Tgt Ion: 136 Resp: 90191
Ion Ratio Lower Upper
136 100
137 11.0 8.7 13.1
54 7.5 6.2 9.2
68 5.6 4.2 6.4


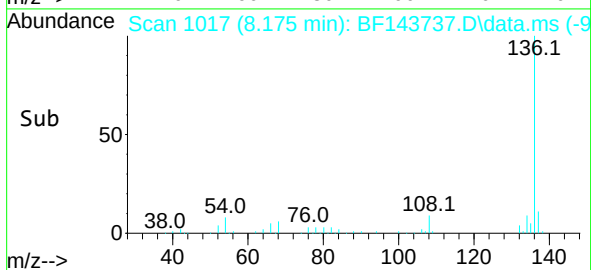
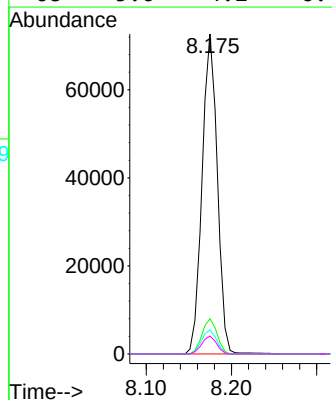
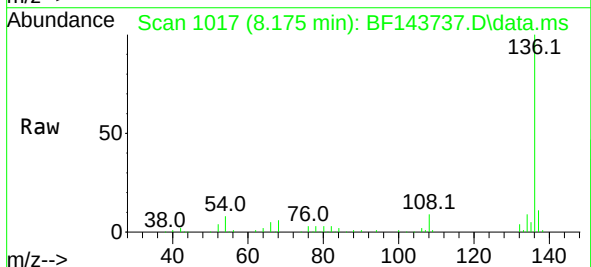


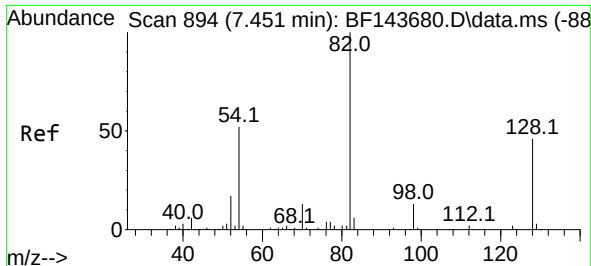

#23
Nitrobenzene-d5
Concen: 105.865 ng
RT: 7.451 min Scan# 894
Delta R.T. -0.000 min
Lab File: BF143737.D
Acq: 12 Sep 2025 17:09




Instrument :
BNA_F
ClientSampleId :
MH-384


Tgt Ion: 82 Resp: 153504
Ion Ratio Lower Upper
82 100
128 47.0 37.0 55.4
54 50.4 41.8 62.8

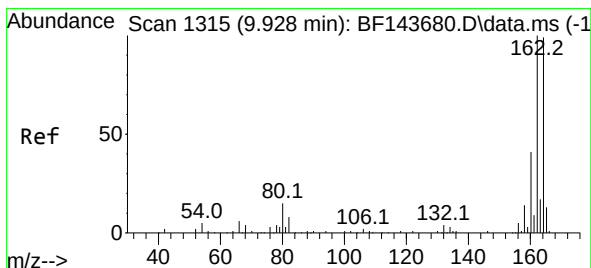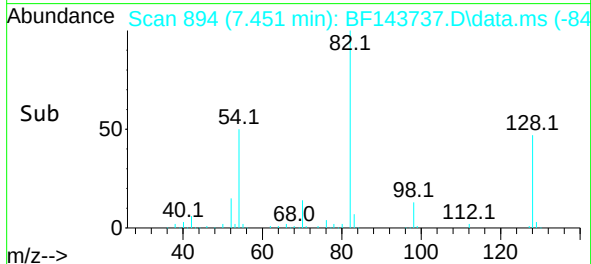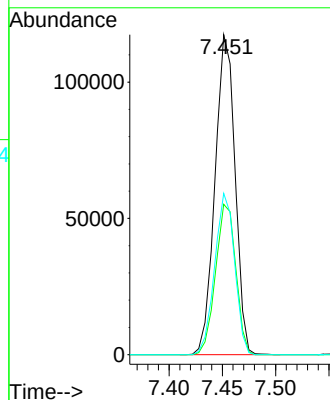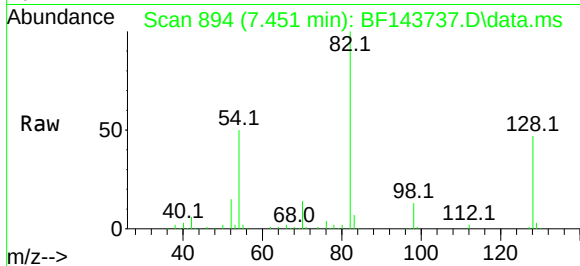

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.933 min Scan# 1316
Delta R.T. 0.006 min
Lab File: BF143737.D
Acq: 12 Sep 2025 17:09


Tgt Ion: 164 Resp: 42668
Ion Ratio Lower Upper
164 100
162 100.3 80.6 121.0
160 41.6 33.0 49.4

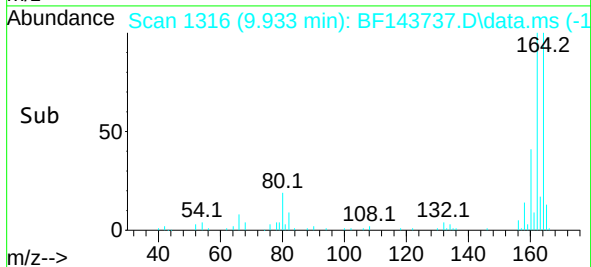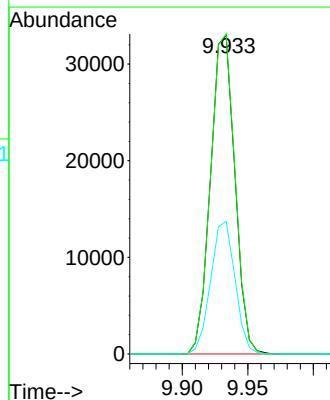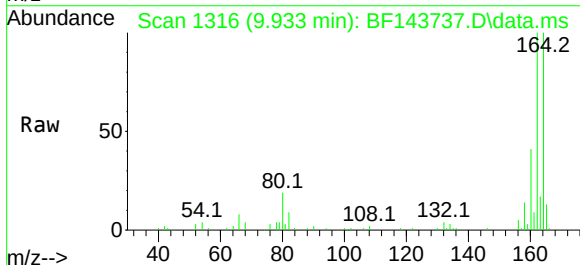



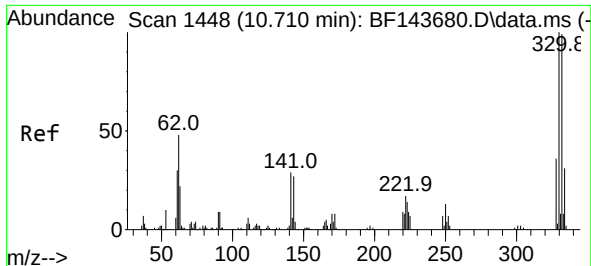


#42
2,4,6-Tribromophenol
Concen: 147.010 ng
RT: 10.722 min Scan# 1448
Delta R.T. 0.012 min
Lab File: BF143737.D
Acq: 12 Sep 2025 17:09

Instrument :
BNA_F
ClientSampleId :
MH-384



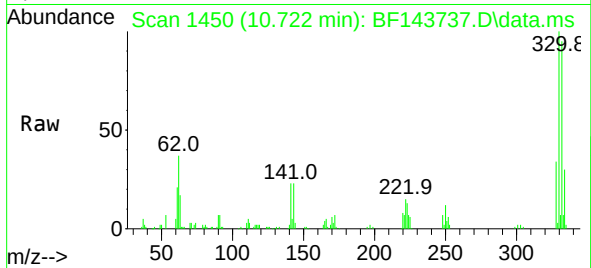



Tgt Ion:330 Resp: 63214
Ion Ratio Lower Upper
330 100
332 95.3 79.2 118.8
141 25.5 22.2 33.4

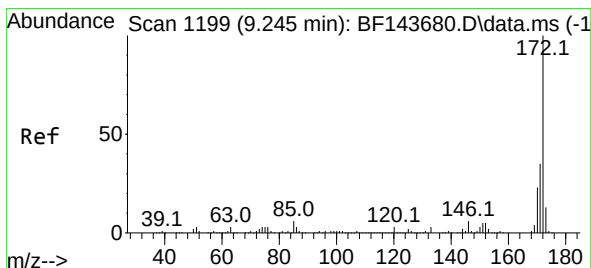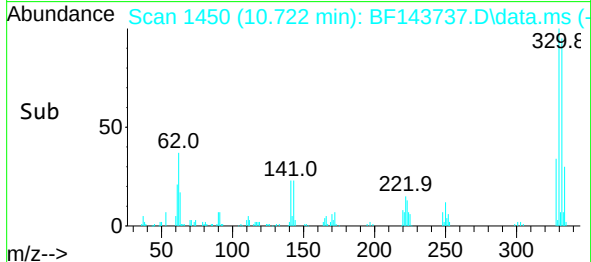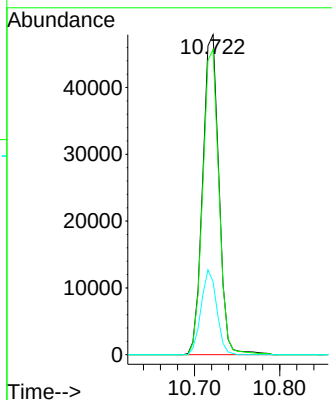

#45
2-Fluorobiphenyl
Concen: 112.592 ng
RT: 9.251 min Scan# 1200
Delta R.T. 0.006 min
Lab File: BF143737.D
Acq: 12 Sep 2025 17:09

Tgt Ion:172 Resp: 318022
Ion Ratio Lower Upper
172 100
171 35.3 27.9 41.9
170 22.9 18.6 27.8

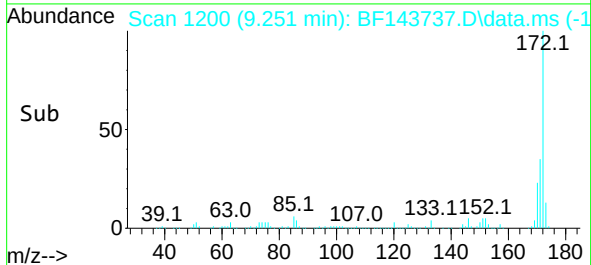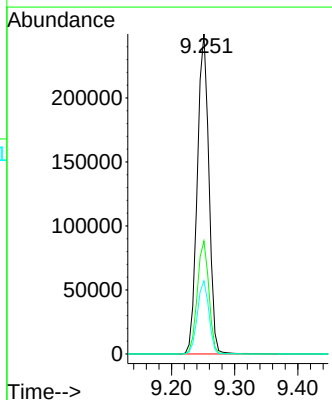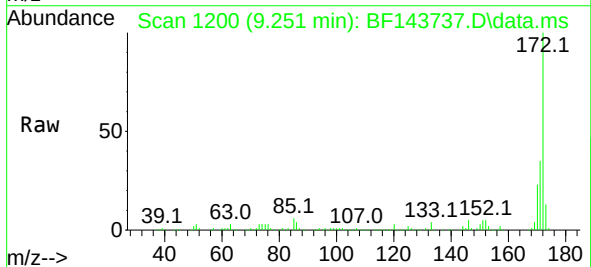

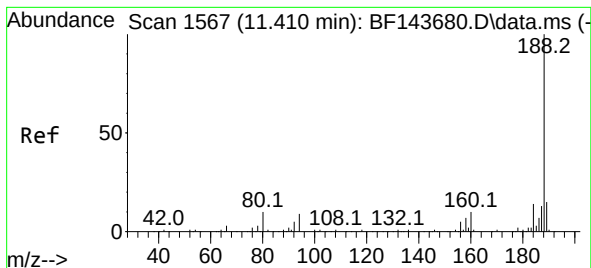

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.416 min Scan# 1

Delta R.T. 0.006 min

Lab File: BF143737.D

Acq: 12 Sep 2025 17:09

Instrument :

BNA_F

ClientSampleId :

MH-384





Tgt Ion:188 Resp: 68736

Ion Ratio Lower Upper

188 100

94 10.1 7.4 11.0

80 10.4 7.7 11.5

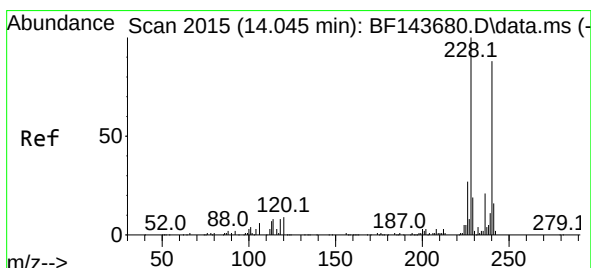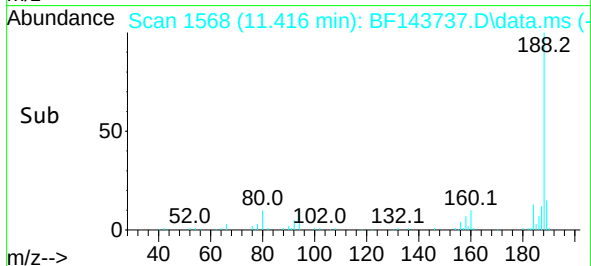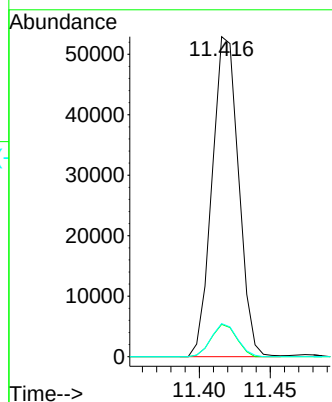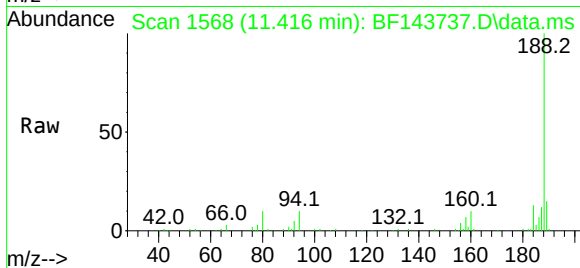

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.057 min Scan# 2017

Delta R.T. 0.012 min

Lab File: BF143737.D

Acq: 12 Sep 2025 17:09




Tgt Ion:240 Resp: 73789


Ion Ratio Lower Upper

240 100

120 10.9 8.4 12.6

236 24.8 18.6 28.0

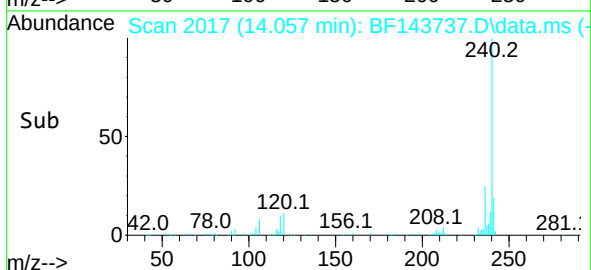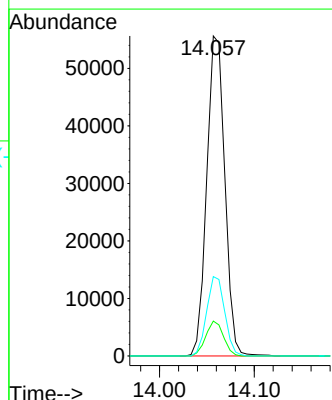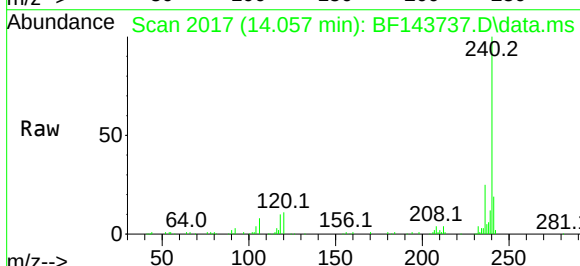

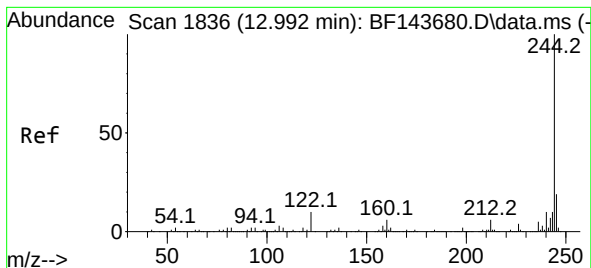

#79

Terphenyl-d14

Concen: 77.984 ng

RT: 13.010 min Scan# 1

Delta R.T. 0.018 min

Lab File: BF143737.D

Acq: 12 Sep 2025 17:09

Instrument :

BNA_F

ClientSampleId :

MH-384





Tgt Ion:244 Resp: 355092

Ion Ratio Lower Upper

244 100

212 6.1 5.0 7.6

122 10.3 7.9 11.9

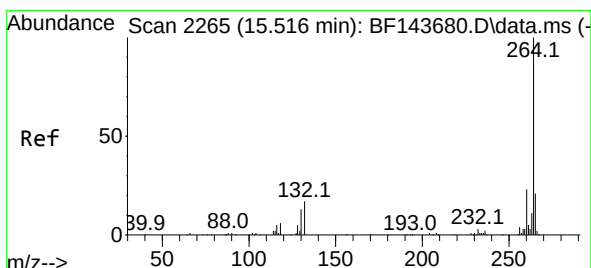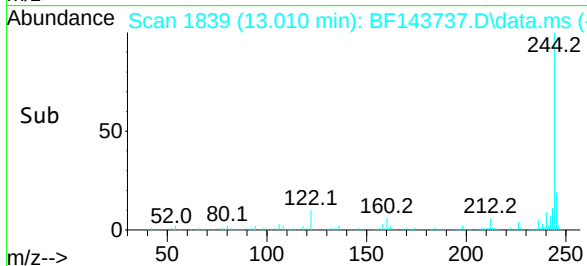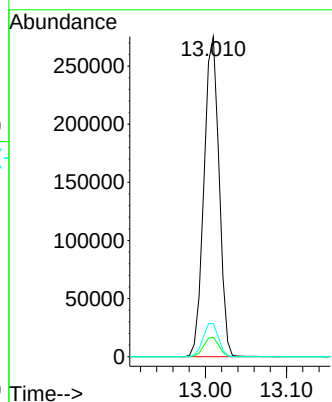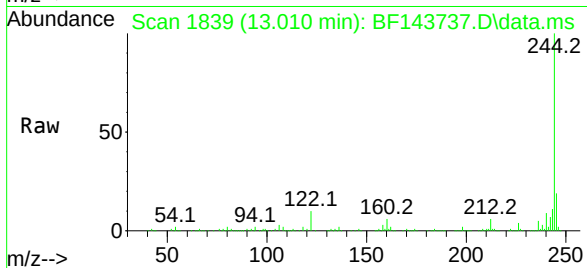

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.545 min Scan# 2270

Delta R.T. 0.029 min

Lab File: BF143737.D

Acq: 12 Sep 2025 17:09

Tgt Ion:264 Resp: 71747

Ion Ratio Lower Upper

264 100

260 23.7 18.4 27.6

265 22.3 17.1 25.7

