
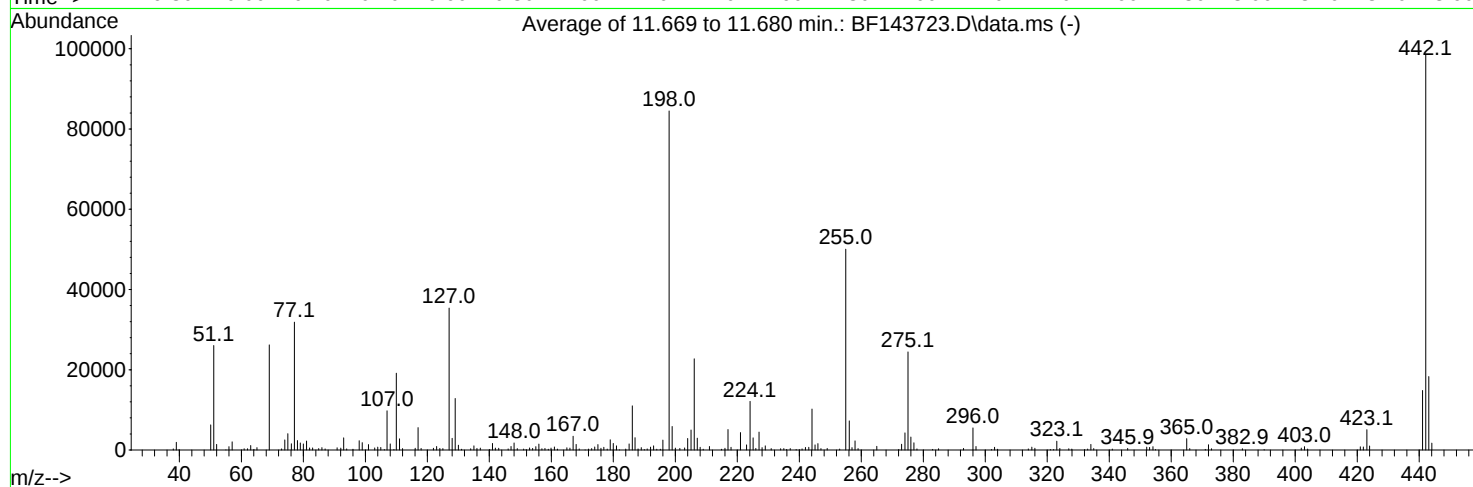


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091225\
Data File : BF143723.D
Acq On : 12 Sep 2025 10:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Sep 09 15:20:16 2025

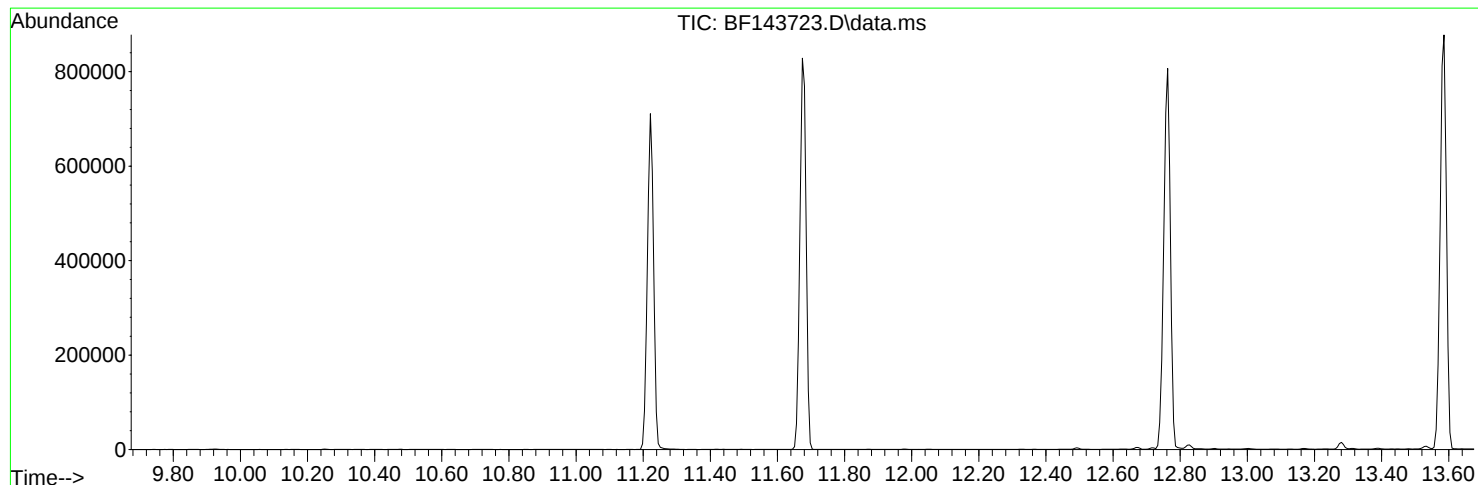

AutoFind: Scans 1611, 1612, 1613; Background Corrected with Scan 1605

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	26219	PASS
70	69	0.00	2	0.0	0	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	84485	PASS
199	198	5	9	6.9	5864	PASS
365	198	1	100	3.3	2825	PASS
441	443	0.01	150	81.0	14822	PASS
442	442	100	100	100.0	98405	PASS
443	442	15	24	18.6	18297	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
9/12/2025	BNA_F	<u>BF143723.D</u>
Compound Name	Response	Retention Time
DDT	247448	13.568
DDD	6010	13.28
DDE	265	12.945
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6275	253723	2.47

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091225\
Data File : BF143723.D
Acq On : 12 Sep 2025 10:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 12 10:45:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 15:20:16 2025
Response via : Initial Calibration

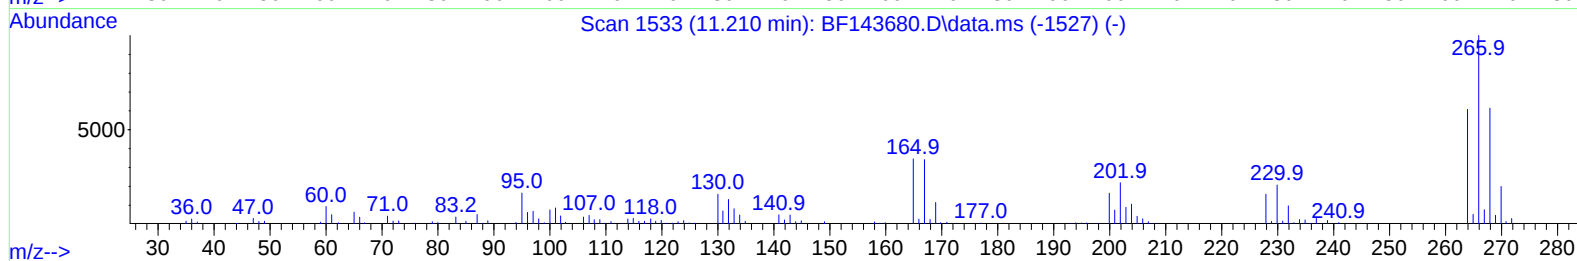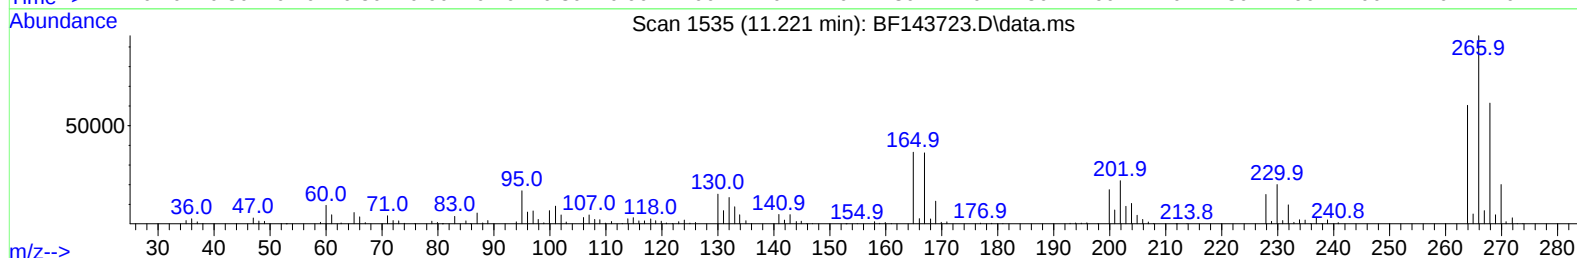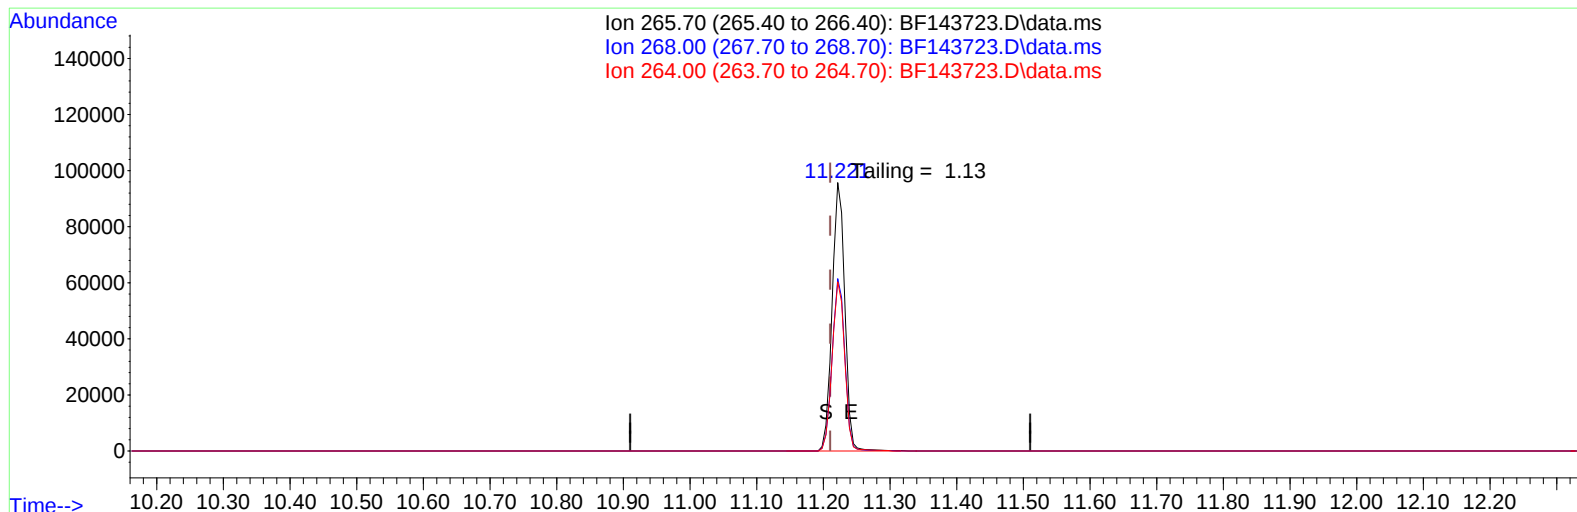

TIC: BF143723.D\data.ms

(70) Pentachlorophenol (C)

11.221min (+ 0.011) 36182.88 ng




response 126443

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	64.23
264.00	60.80	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF091225\
Data File : BF143723.D
Acq On : 12 Sep 2025 10:14
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 12 10:45:24 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 09 15:20:16 2025
Response via : Initial Calibration

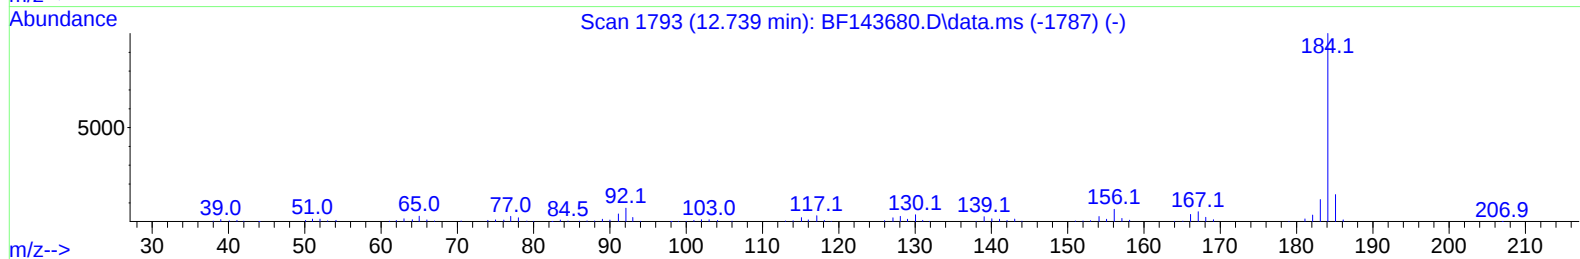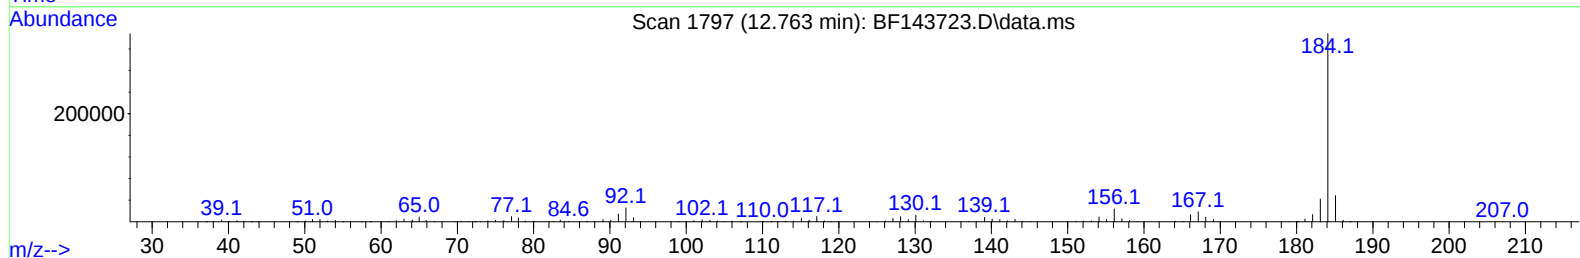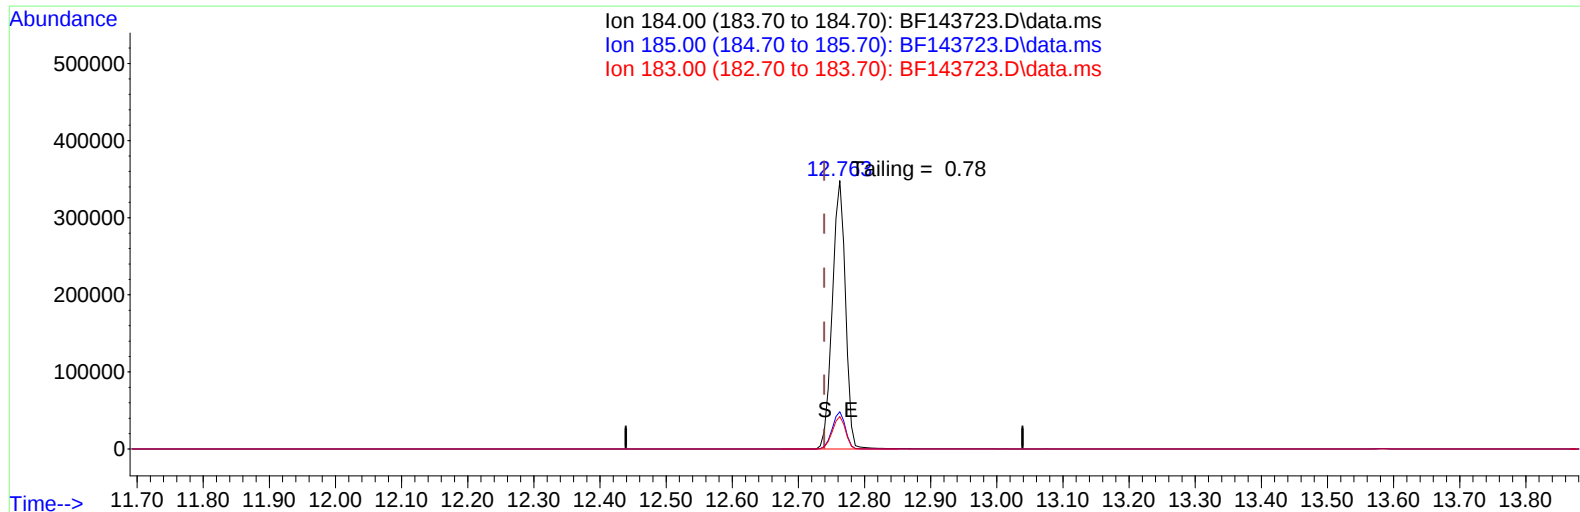

TIC: BF143723.D\data.ms

(77) Benzidine

12.763min (+ 0.023) 61529.69 ng

response 483562

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.92
183.00	11.80	12.11
0.00	0.00	0.00