
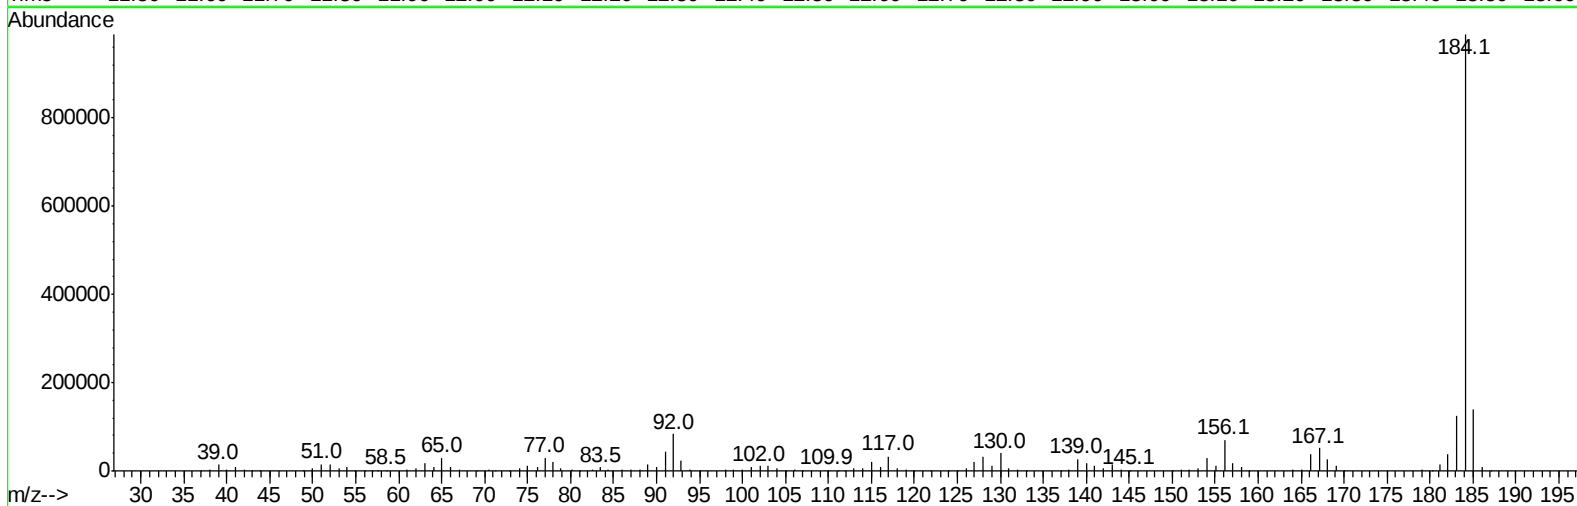


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF091317\
 Data File : BF098481.D
 Acq On : 13 Sep 2017 10:59
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 08:12:35 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Sep 12 02:14:50 2017
 Response via : Initial Calibration

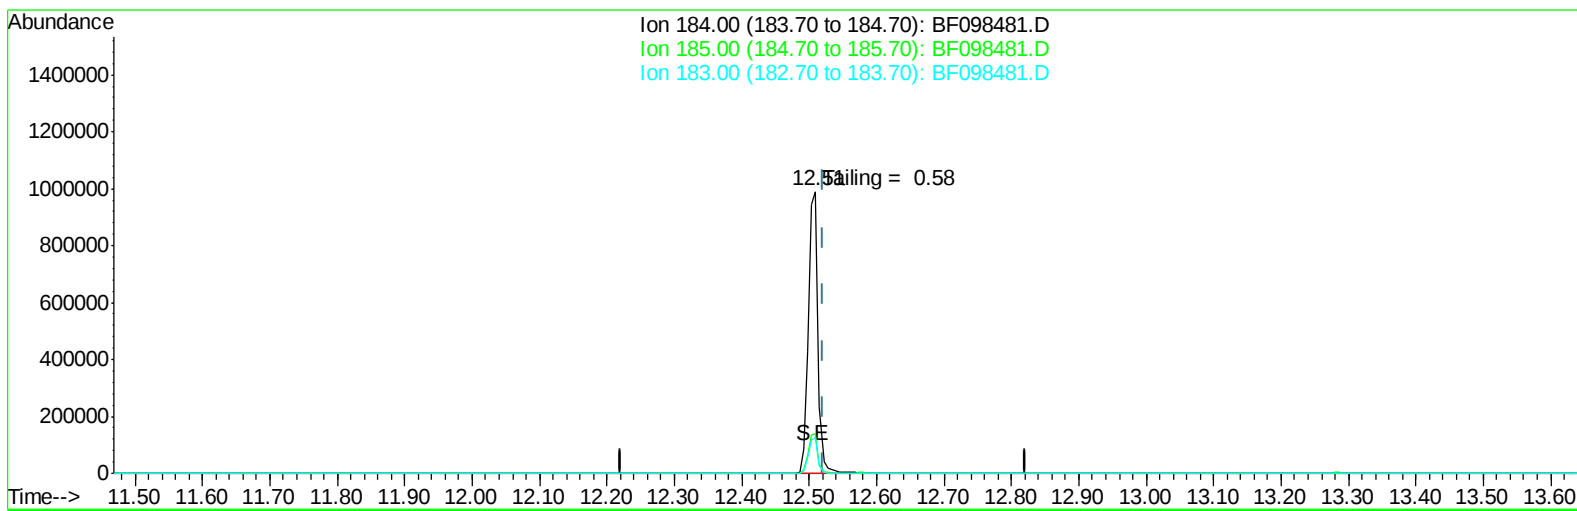

TIC: BF098481.D

(76) Benzidine



12.510min (-0.012) 0.00ng

response 987989

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.16#
183.00	12.20	12.53
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF091317\
Data File : BF098481.D
Acq On : 13 Sep 2017 10:59
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 08:12:35 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

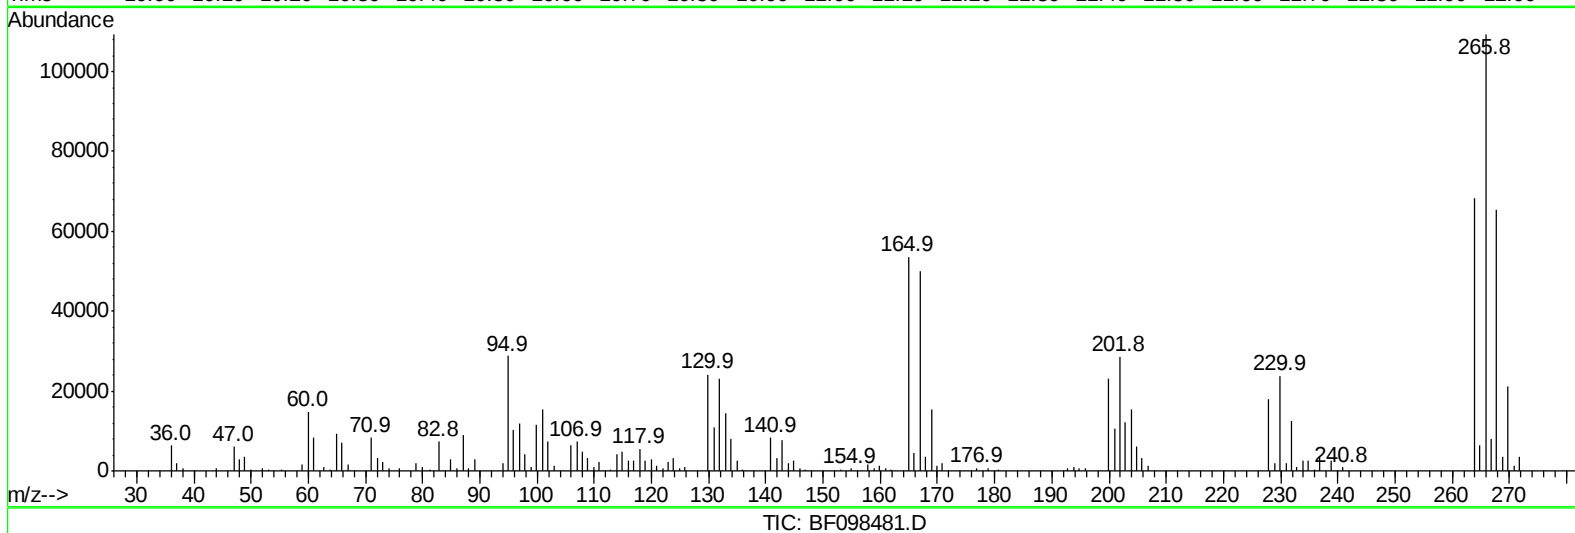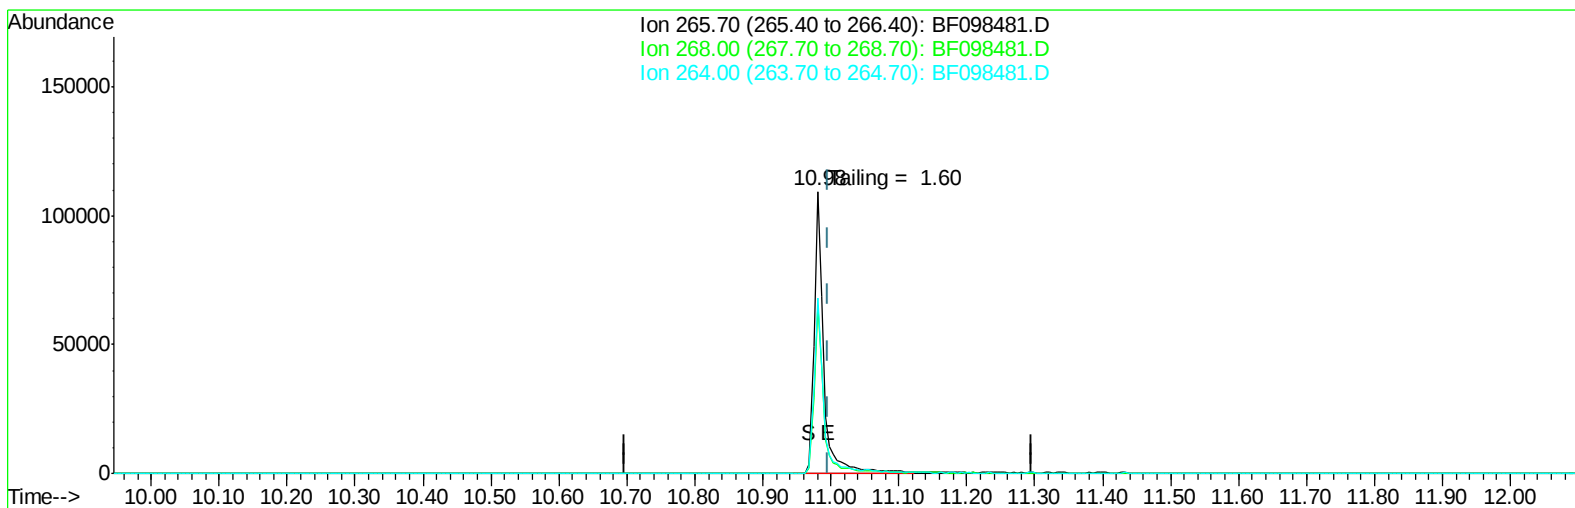

(69) Pentachlorophenol (C)

10.980min (-0.017) 39850.02ng

response 106902

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.77
264.00	64.60	62.39
0.00	0.00	0.00