
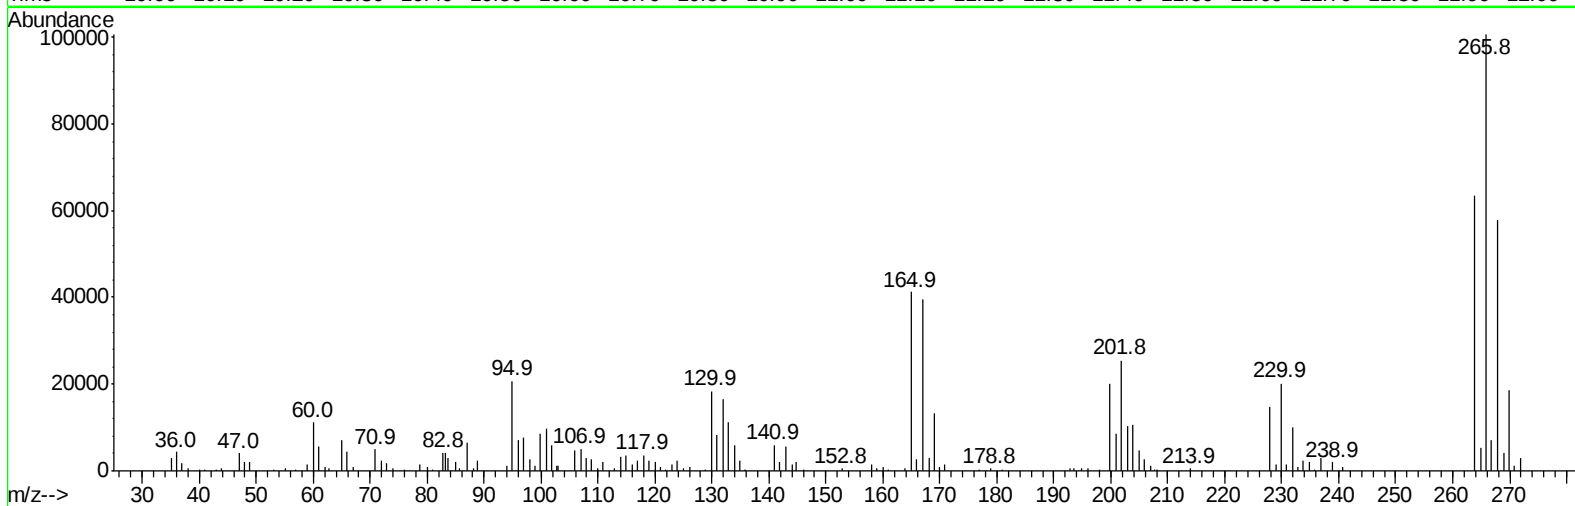


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF091317\
Data File : BF098492.D
Acq On : 13 Sep 2017 16:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 08:13:37 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

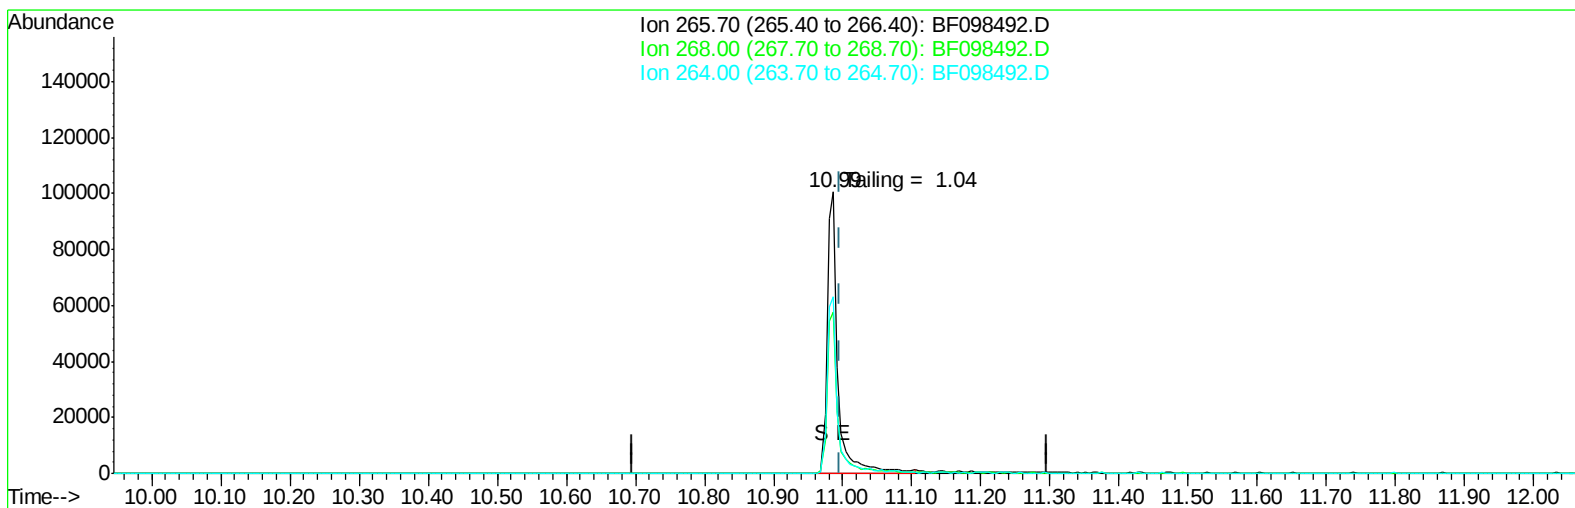

TIC: BF098492.D

(69) Pentachlorophenol (C)



10.986min (-0.011) 34416.84ng

response 106454

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	57.42
264.00	64.60	62.93
0.00	0.00	0.00

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF091317\
Data File : BF098492.D
Acq On : 13 Sep 2017 16:17
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 14 08:13:37 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 12 02:14:50 2017
Response via : Initial Calibration

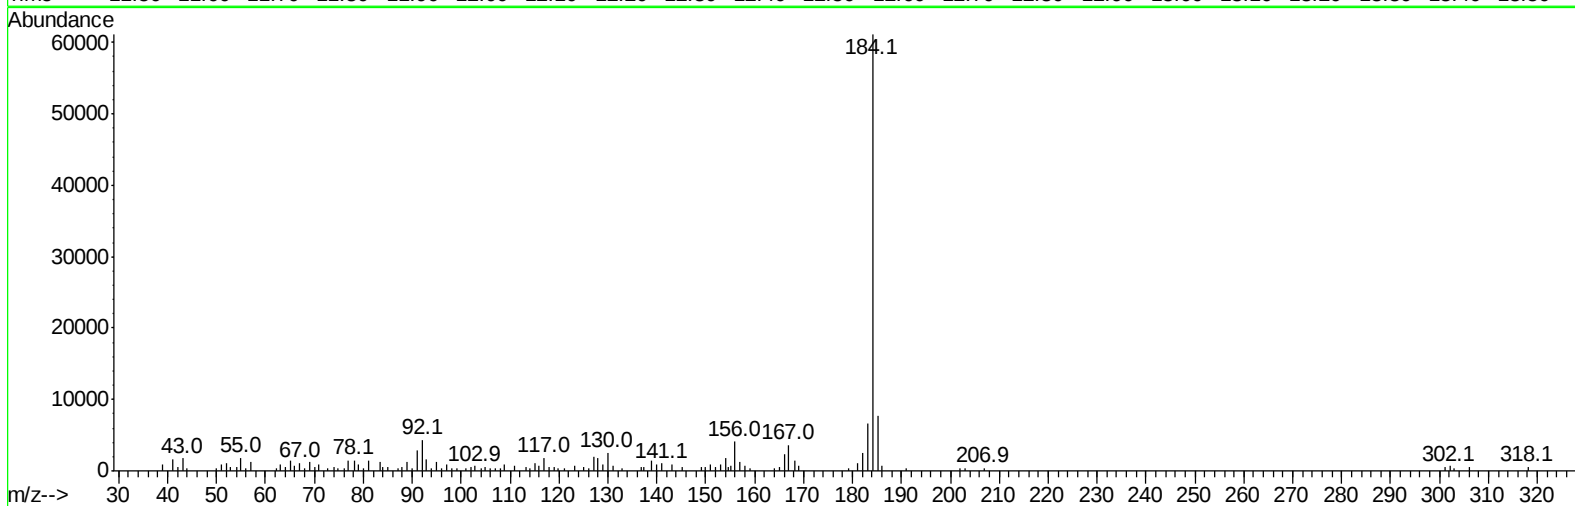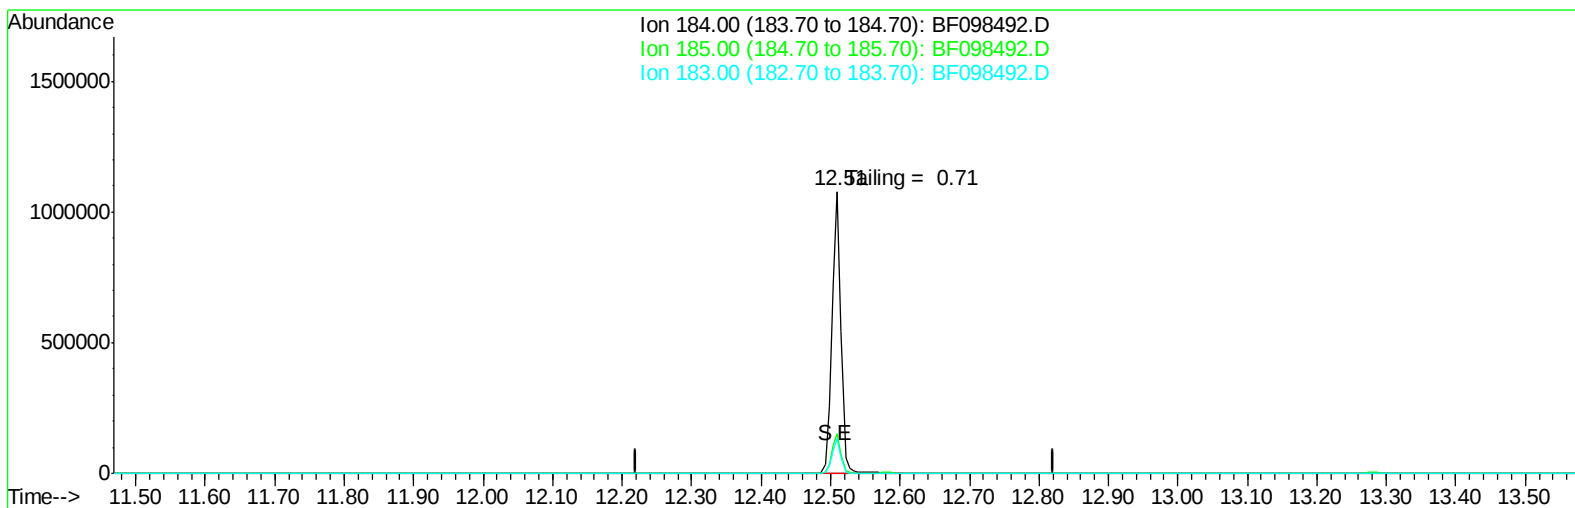

TIC: BF098492.D

(76) Benzidine

12.521min (-12.521) 0.00ng

response 0

Ion	Exp%	Act%
184.00	100	0.00
185.00	19.40	0.00#
183.00	12.20	0.00#
0.00	0.00	0.00