

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF091317\
 Data File : BF098490.D
 Acq On : 13 Sep 2017 15:18
 Operator : SJ/JU
 Sample : I5208-10 5X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 CL-02-091117-D

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.816	461	464	476	rBV	56999	82742	5.57%	0.585%
2	5.257	535	539	551	rBV	710253	841659	56.64%	5.955%
3	6.298	713	716	726	rBV	862510	868944	58.48%	6.148%
4	6.422	734	737	747	rBV	1044517	878811	59.14%	6.218%
5	6.651	773	776	788	rBV	1334670	1099993	74.03%	7.783%
6	6.804	799	802	812	rVB	662813	636803	42.86%	4.506%
7	7.216	869	872	886	rBV	498791	505884	34.04%	3.579%
8	7.939	990	995	998	rBV	1583427	1453287	97.80%	10.282%
9	9.010	1173	1177	1182	rBV	1172419	932142	62.73%	6.595%
10	9.410	1242	1245	1248	rVB	160694	118183	7.95%	0.836%
11	9.545	1264	1268	1274	rBV	22661	21497	1.45%	0.152%
12	9.686	1288	1292	1297	rBV	1729127	1485942	100.00%	10.513%
13	10.475	1422	1426	1433	rBV	458524	405668	27.30%	2.870%
14	10.592	1443	1446	1451	rBV4	13896	19216	1.29%	0.136%
15	11.169	1540	1544	1547	rBV	1447069	1327689	89.35%	9.394%
16	11.698	1631	1634	1637	rVB	17989	17604	1.18%	0.125%
17	11.774	1644	1647	1650	rBV3	20274	21808	1.47%	0.154%
18	11.869	1658	1663	1665	rBV5	13320	16958	1.14%	0.120%
19	12.216	1719	1722	1725	rBV4	28559	30120	2.03%	0.213%
20	12.257	1726	1729	1733	rVB4	19134	24676	1.66%	0.175%
21	12.374	1745	1749	1755	rBV	166187	147828	9.95%	1.046%
22	12.468	1763	1765	1770	rBV3	19157	25971	1.75%	0.184%
23	12.604	1782	1788	1790	rBV	155584	157958	10.63%	1.118%
24	12.657	1794	1797	1802	rVB7	14938	18670	1.26%	0.132%
25	12.745	1809	1812	1816	rBV	788070	664312	44.71%	4.700%
26	12.821	1822	1825	1829	rVB6	14949	22994	1.55%	0.163%
27	13.033	1858	1861	1866	rBV5	26159	29017	1.95%	0.205%
28	13.651	1963	1966	1970	rBV2	45607	45259	3.05%	0.320%
29	13.798	1987	1991	1994	rBV	1190538	1126440	75.81%	7.970%
30	14.804	2160	2162	2165	rBV	86828	91929	6.19%	0.650%
31	15.198	2224	2229	2236	rVB	821116	1013664	68.22%	7.172%


Sum of corrected areas: 14133668

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF091317\
Data File : BF098490.D
Acq On : 13 Sep 2017 15:18
Operator : SJ/JU
Sample : I5208-10 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-091117-D

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

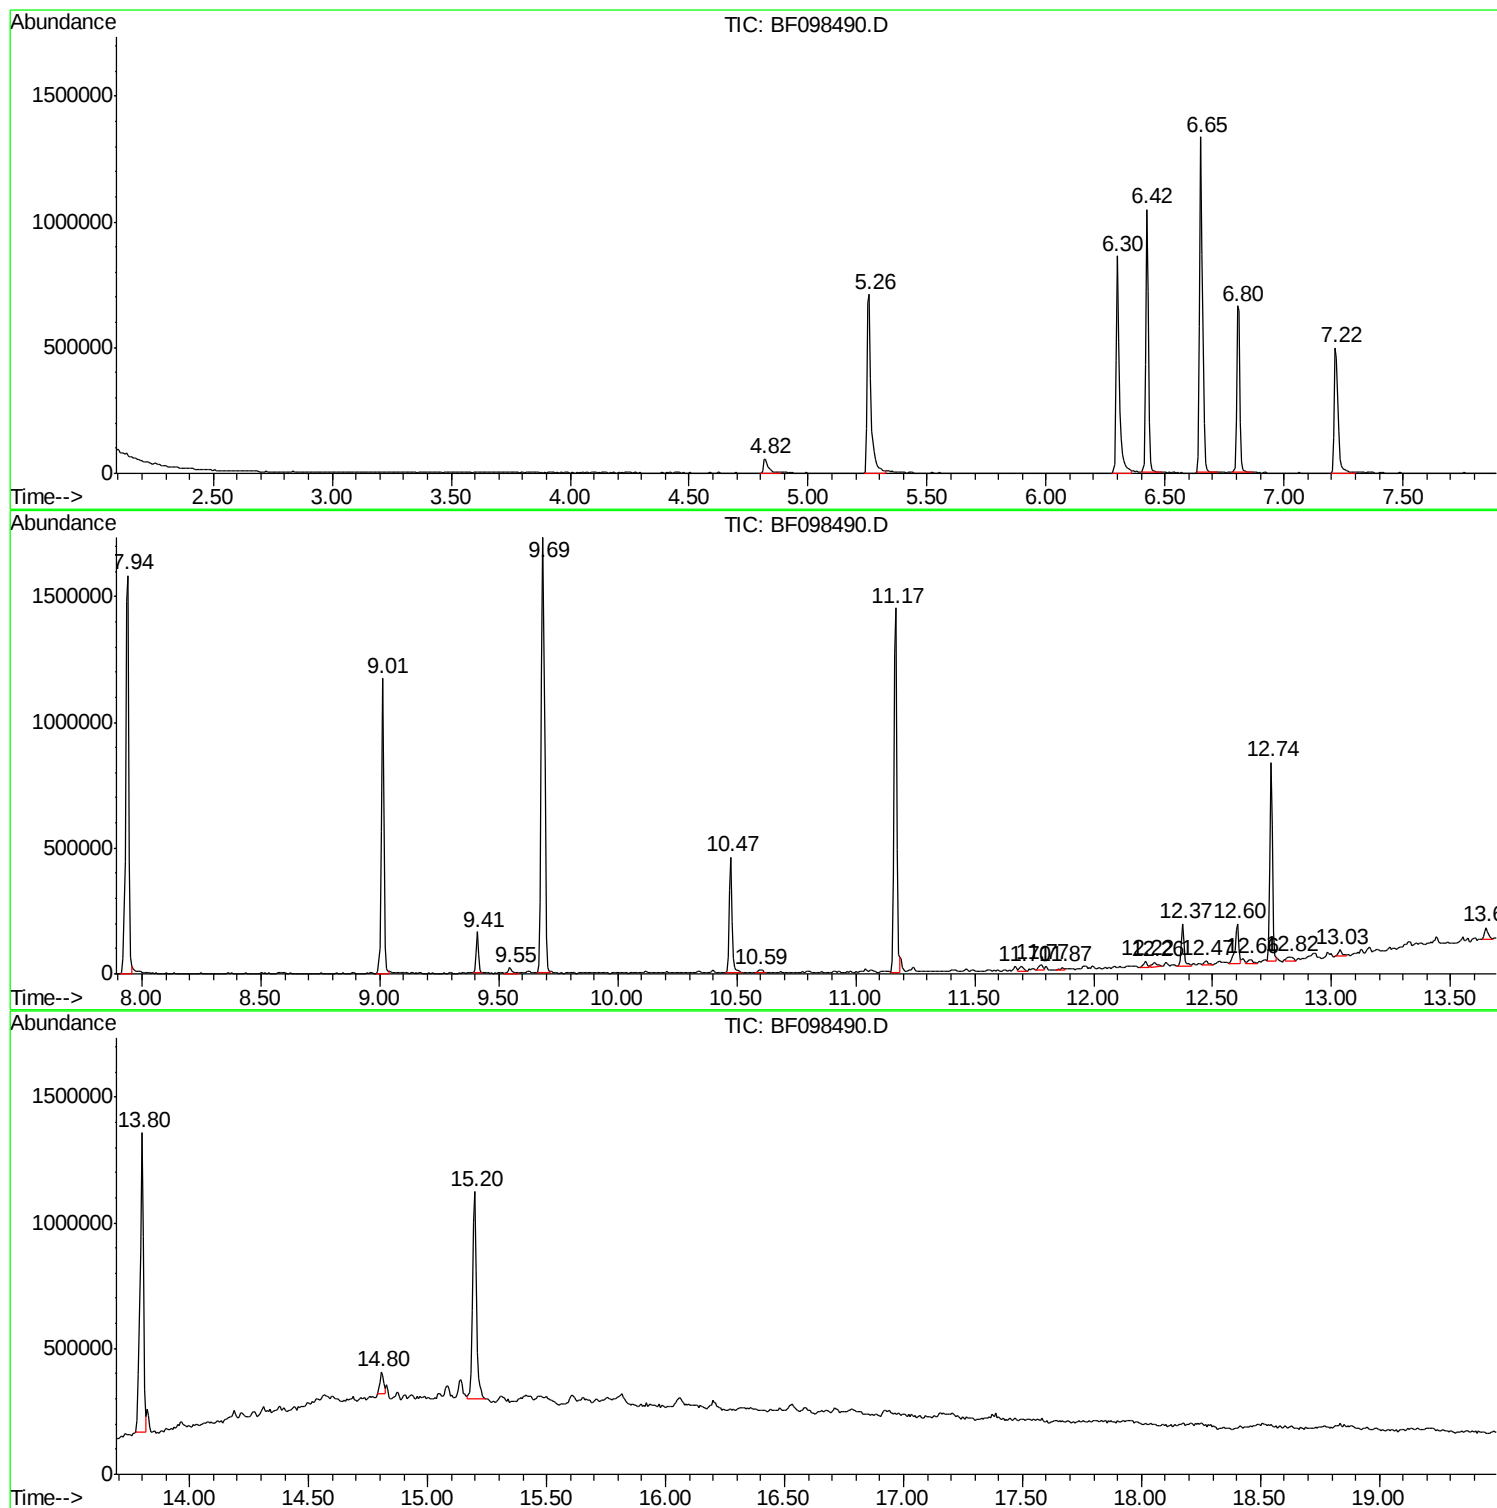

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF091317\
Data File : BF098490.D
Acq On : 13 Sep 2017 15:18
Operator : SJ/JU
Sample : I5208-10 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-091117-D










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.42 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.42	15.98 ng	878811	1,4-Dichlorobenzene-d4	6.65

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	16
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9

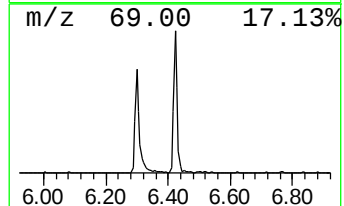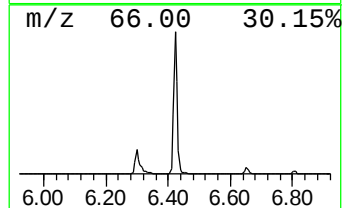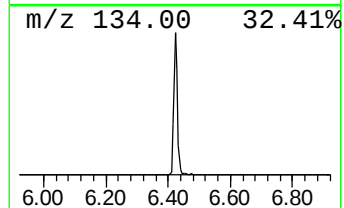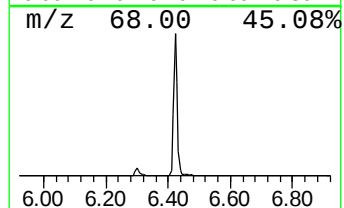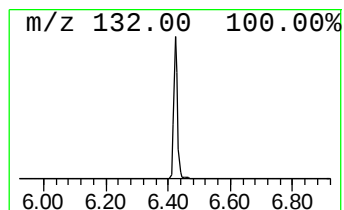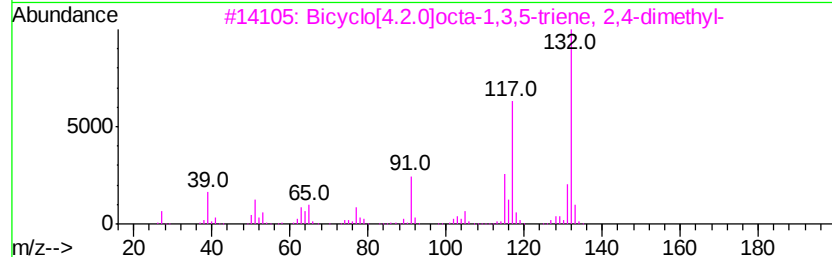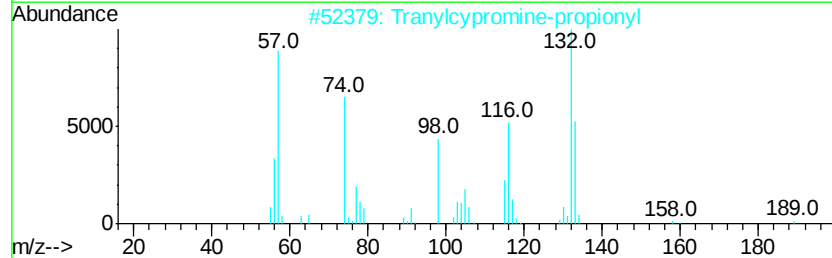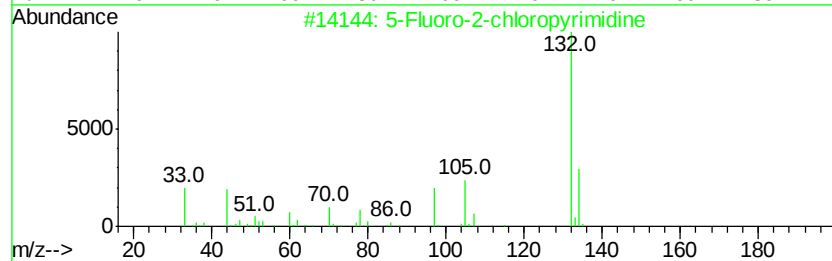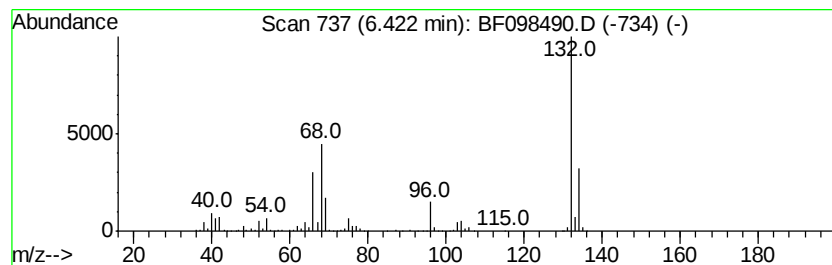

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF091317\
Data File : BF098490.D
Acq On : 13 Sep 2017 15:18
Operator : SJ/JU
Sample : I5208-10 5X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
CL-02-091117-D

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.42	6.42	16.0	ng	878811	1	6.65	1099990	20.0