

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF091317\
 Data File : BF098515.D
 Acq On : 14 Sep 2017 3:20
 Operator : SJ/JU
 Sample : I5159-08 10X
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-42-A1

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.828	464	466	472	rBV	12444	17177	1.44%	0.212%
2	5.263	537	540	554	rBV	212154	276839	23.18%	3.418%
3	6.310	715	718	735	rBV	242601	320382	26.82%	3.956%
4	6.428	735	738	745	rVV	302084	287679	24.09%	3.552%
5	6.657	773	777	784	rBV	1039999	946065	79.21%	11.682%
6	6.810	799	803	815	rVB	269516	235775	19.74%	2.911%
7	7.222	870	873	882	rBV	143511	146304	12.25%	1.807%
8	7.939	991	995	1005	rBV	1450260	1194346	100.00%	14.747%
9	8.504	1087	1091	1094	rBV	15772	17134	1.43%	0.212%
10	9.010	1174	1177	1184	rBV	355301	308855	25.86%	3.814%
11	9.410	1243	1245	1251	rVB	68048	57089	4.78%	0.705%
12	9.686	1289	1292	1297	rVB	1164309	1050290	87.94%	12.969%
13	10.398	1410	1413	1417	rBV	73089	64238	5.38%	0.793%
14	10.480	1424	1427	1433	rBV	116434	106375	8.91%	1.313%
15	10.604	1443	1448	1451	rVB3	20396	28170	2.36%	0.348%
16	11.169	1540	1544	1548	rBV	1087728	913241	76.46%	11.276%
17	11.421	1583	1587	1591	rBV4	8454	15051	1.26%	0.186%
18	12.221	1720	1723	1725	rBV3	24083	24062	2.01%	0.297%
19	12.380	1747	1750	1753	rBV	61637	52330	4.38%	0.646%
20	12.610	1784	1789	1791	rBV	78781	96320	8.06%	1.189%
21	12.751	1809	1813	1816	rBV	304060	265653	22.24%	3.280%
22	13.186	1885	1887	1891	rBV4	33556	33731	2.82%	0.417%
23	13.804	1988	1992	1996	rBV	1040231	955855	80.03%	11.803%
24	15.204	2227	2230	2236	rVB	558590	685715	57.41%	8.467%


Sum of corrected areas: 8098676

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF091317\
Data File : BF098515.D
Acq On : 14 Sep 2017 3:20
Operator : SJ/JU
Sample : I5159-08 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-42-A1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

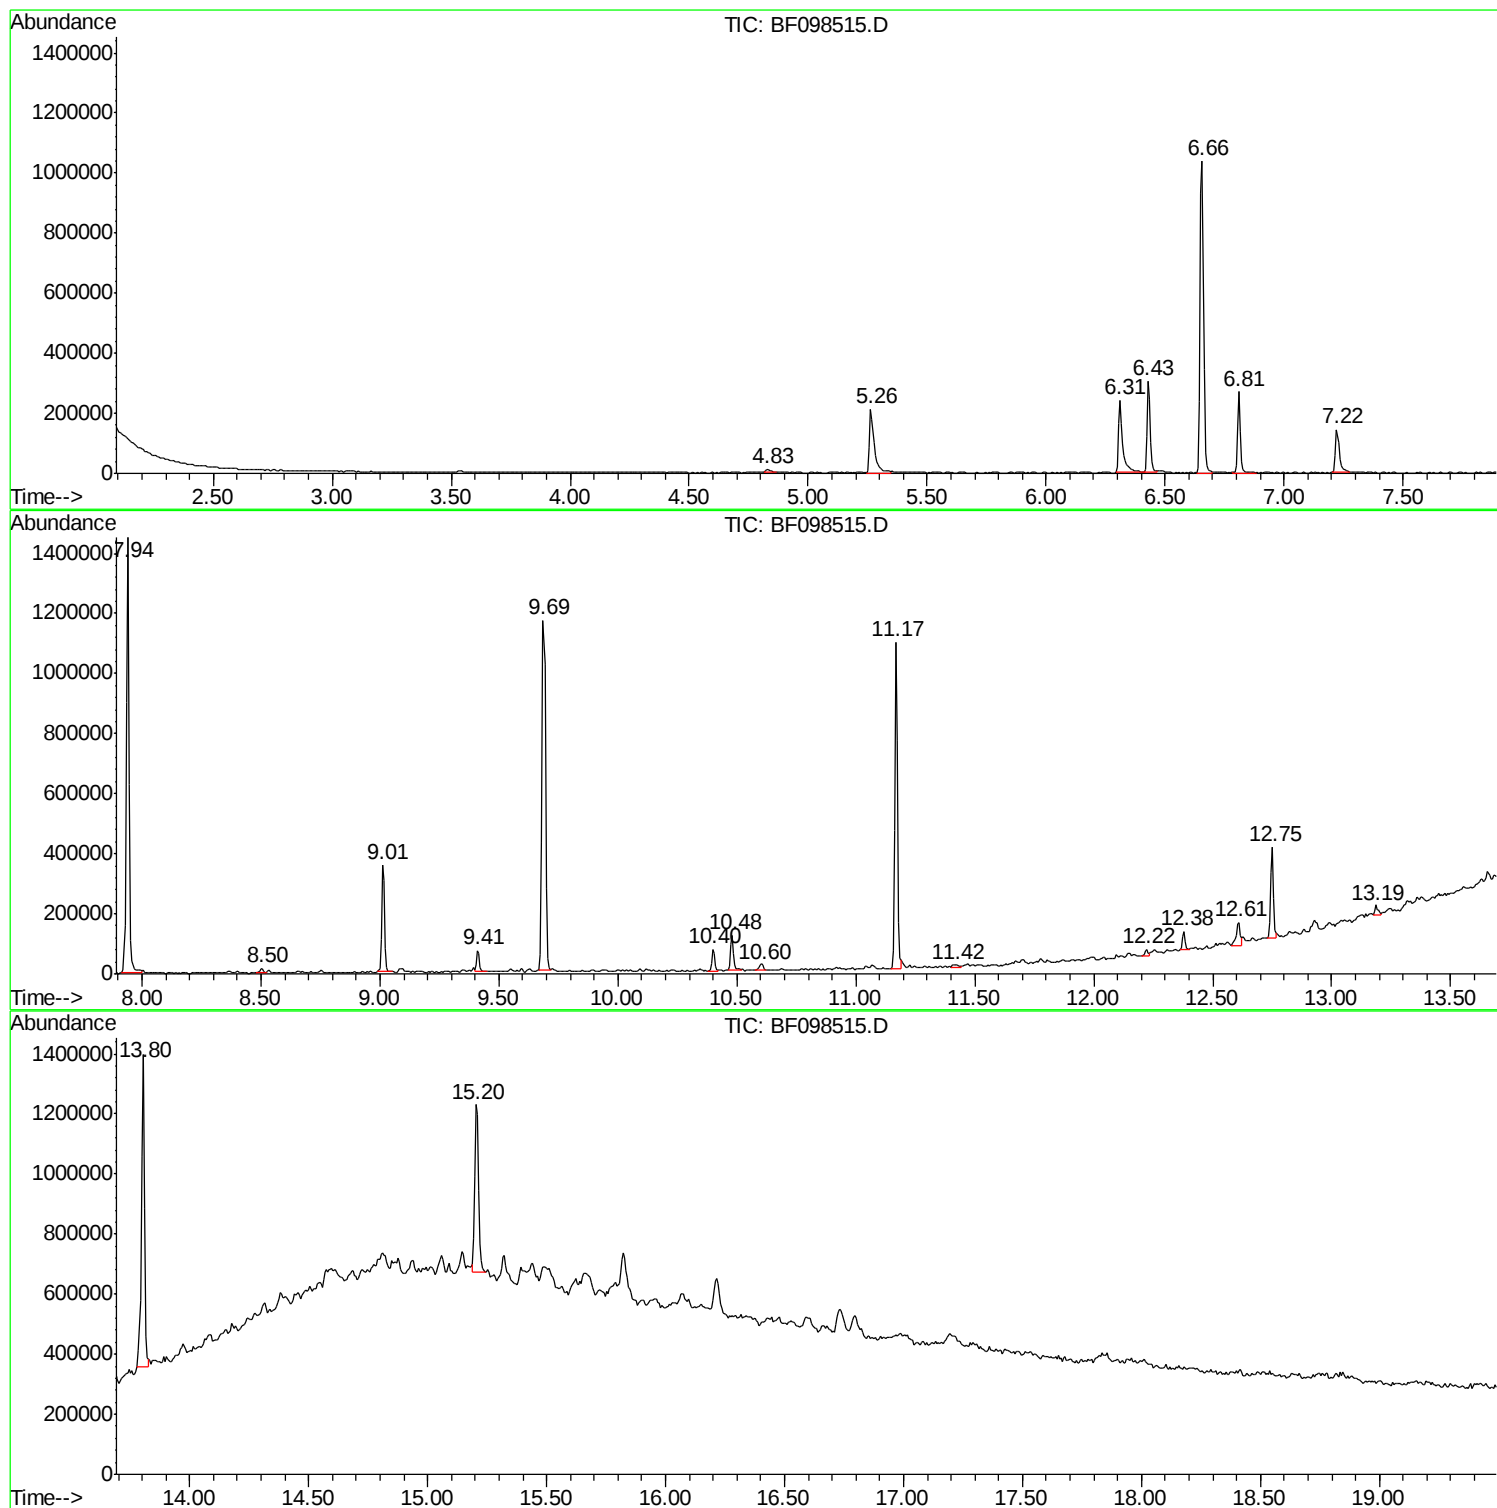

Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA F\DATA\BF091317\
Data File : BF098515.D
Acq On : 14 Sep 2017 3:20
Operator : SJ/JU
Sample : I5159-08 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-42-A1










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.43 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.43	6.08 ng	287679	1,4-Dichlorobenzene-d4	6.66

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
3			5-Aminoindole	132	C8H8N2	005192-03-0	12
4			(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	10
5			2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

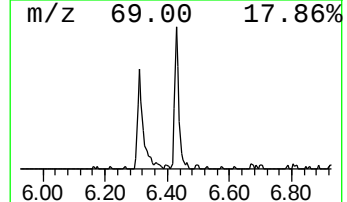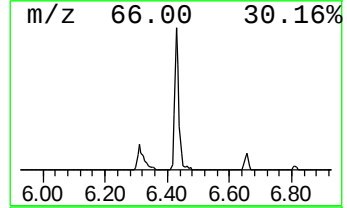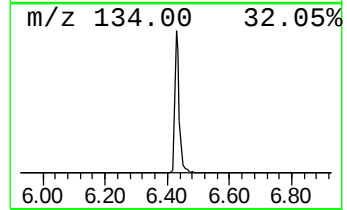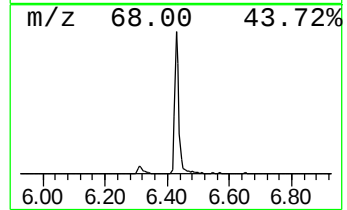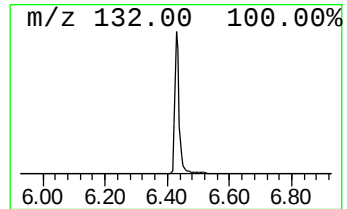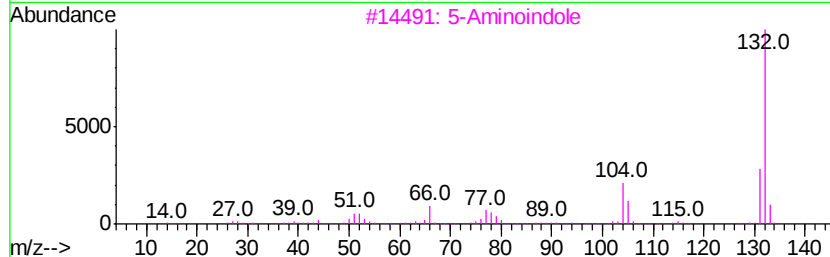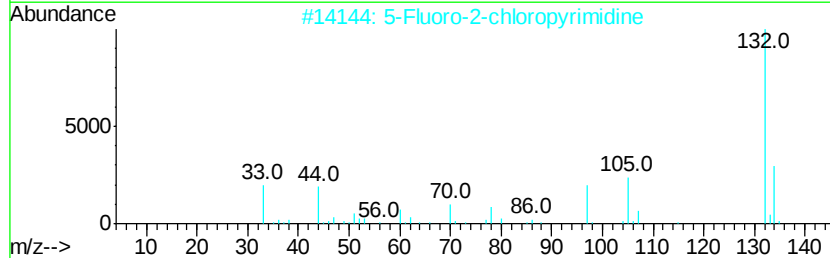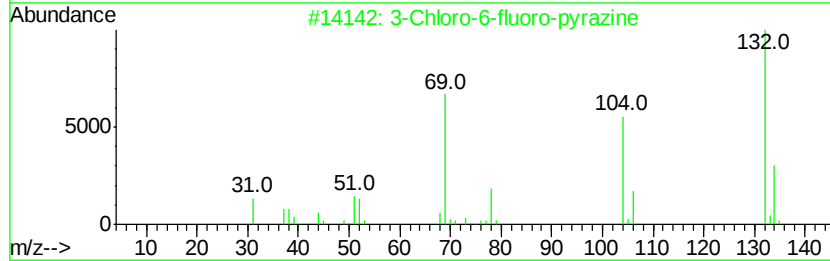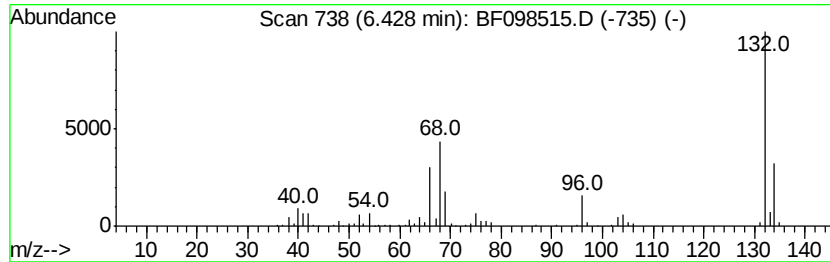

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF091317\
Data File : BF098515.D
Acq On : 14 Sep 2017 3:20
Operator : SJ/JU
Sample : I5159-08 10X
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-42-A1

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.43	6.43	6.1	ng	287679	1	6.66	946065	20.0