

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF091317\
 Data File : BF098516.D
 Acq On : 14 Sep 2017 3:48
 Operator : SJ/JU
 Sample : I5159-10 10X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 G-41-A1-2.5-5

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.828	463	466	475	rBV	14720	23681	1.85%	0.273%
2	5.263	537	540	552	rBV	227548	275647	21.51%	3.180%
3	6.310	714	718	735	rBV	242753	321292	25.07%	3.707%
4	6.428	735	738	744	rBV	338147	306506	23.92%	3.536%
5	6.657	773	777	784	rBV	1028238	955709	74.58%	11.027%
6	6.810	799	803	813	rVB	264237	231288	18.05%	2.669%
7	7.222	870	873	883	rBV	148011	154744	12.08%	1.785%
8	7.939	991	995	1005	rBV	1562834	1281388	100.00%	14.785%
9	8.504	1088	1091	1094	rBV	16651	16924	1.32%	0.195%
10	9.010	1174	1177	1187	rBV	382894	323646	25.26%	3.734%
11	9.410	1240	1245	1249	rVB	64134	62910	4.91%	0.726%
12	9.686	1289	1292	1296	rBV	1391713	1263334	98.59%	14.576%
13	10.345	1401	1404	1408	rVB3	15606	14962	1.17%	0.173%
14	10.398	1410	1413	1417	rBV	70818	61405	4.79%	0.708%
15	10.480	1424	1427	1431	rBV	121388	114091	8.90%	1.316%
16	10.610	1443	1449	1452	rVB2	30204	40900	3.19%	0.472%
17	11.069	1524	1527	1531	rVB	26735	30144	2.35%	0.348%
18	11.169	1541	1544	1548	rBV	1324502	1134007	88.50%	13.084%
19	11.286	1560	1564	1567	rBV6	10495	15674	1.22%	0.181%
20	12.222	1720	1723	1725	rBV3	22278	27437	2.14%	0.317%
21	12.380	1748	1750	1754	rVB	27665	20272	1.58%	0.234%
22	12.751	1810	1813	1820	rVB	304487	273493	21.34%	3.156%
23	13.804	1988	1992	1996	rBV	1052419	934897	72.96%	10.787%
24	15.204	2227	2230	2237	rVB	626506	782648	61.08%	9.030%


Sum of corrected areas: 8666999

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF091317\
Data File : BF098516.D
Acq On : 14 Sep 2017 3:48
Operator : SJ/JU
Sample : I5159-10 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-41-A1-2.5-5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

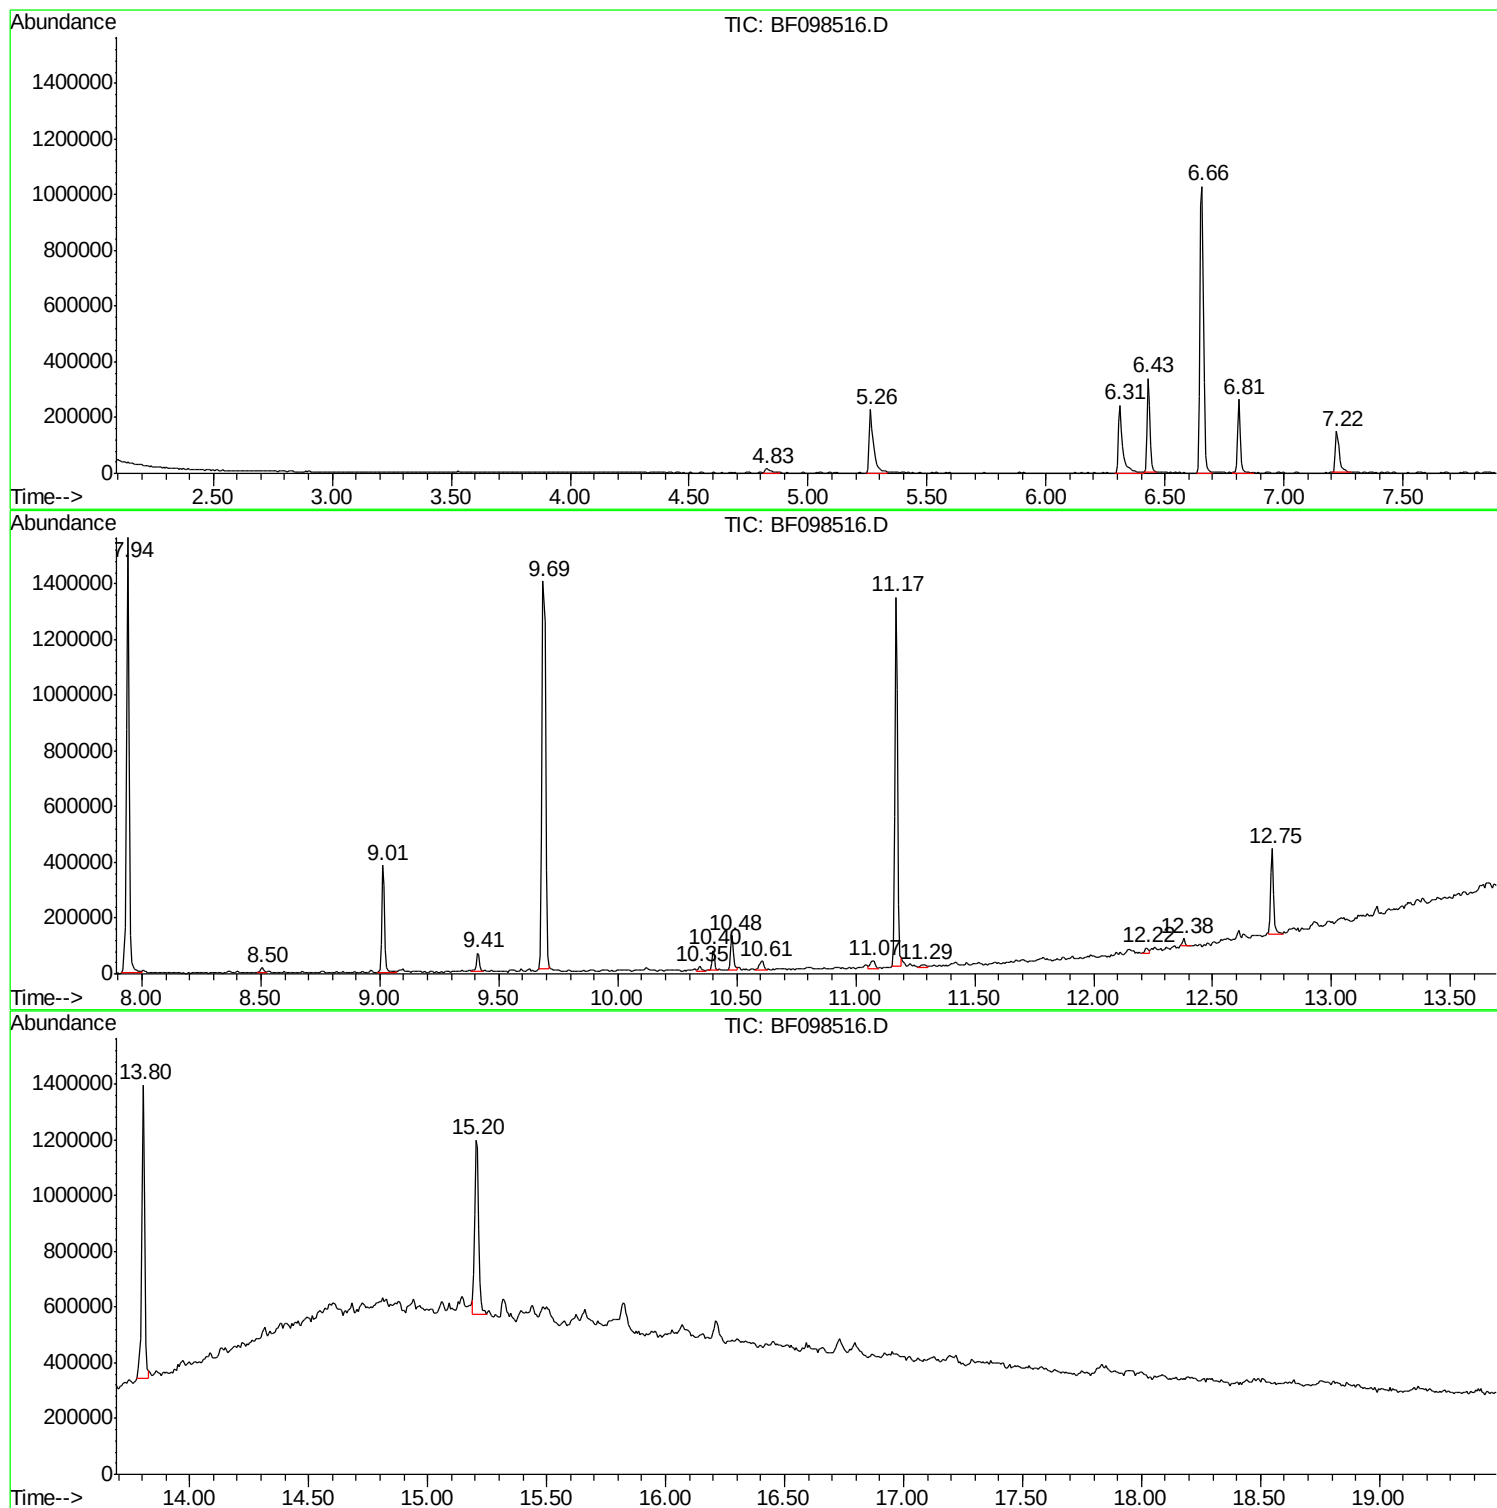

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA F\DATA\BF091317\
Data File : BF098516.D
Acq On : 14 Sep 2017 3:48
Operator : SJ/JU
Sample : I5159-10 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-41-A1-2.5-5










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.43 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.43	6.41 ng	306506	1,4-Dichlorobenzene-d4	6.66

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		(5-Methyl-2-pyridyl)acetonitrile	132	C8H8N2	1000241-93-9	10

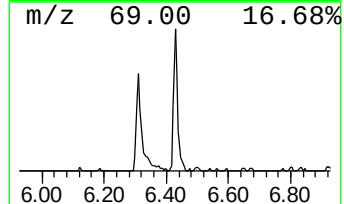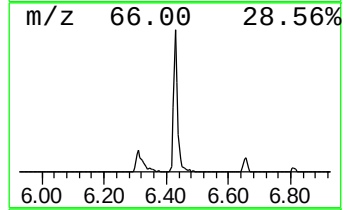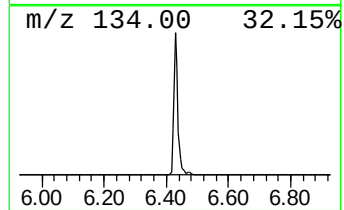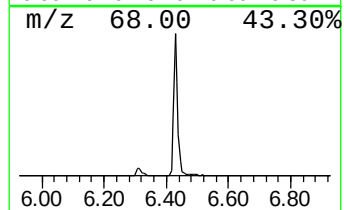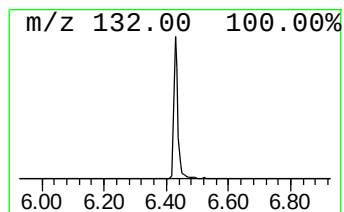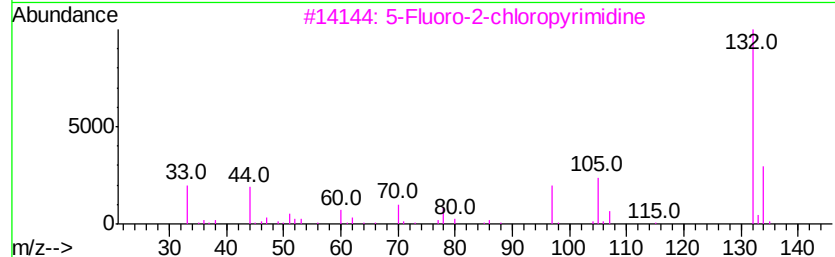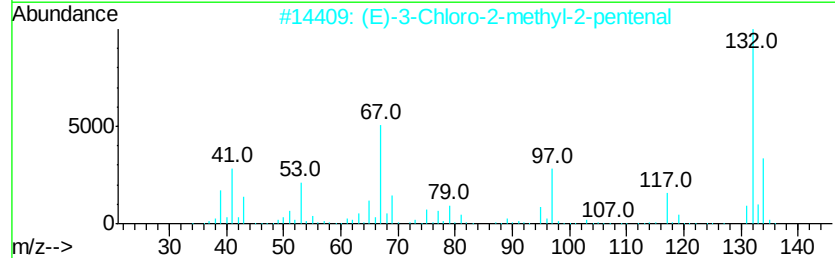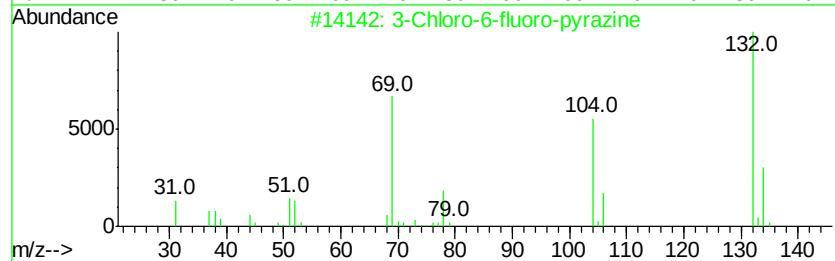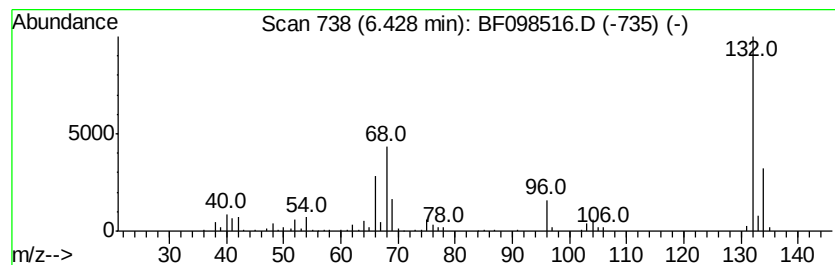

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF091317\
Data File : BF098516.D
Acq On : 14 Sep 2017 3:48
Operator : SJ/JU
Sample : I5159-10 10X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
G-41-A1-2.5-5

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF091117.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.43	6.43	6.4	ng	306506	1	6.66	955709	20.0