


Data Path : \\74.0.250.170\svoasrv\HPCHEM1\BNA F\Data\BF091317\  
 Data File : BF098481.D  
 Acq On : 13 Sep 2017 10:59  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF091117.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Tue Sep 12 02:14:50 2017

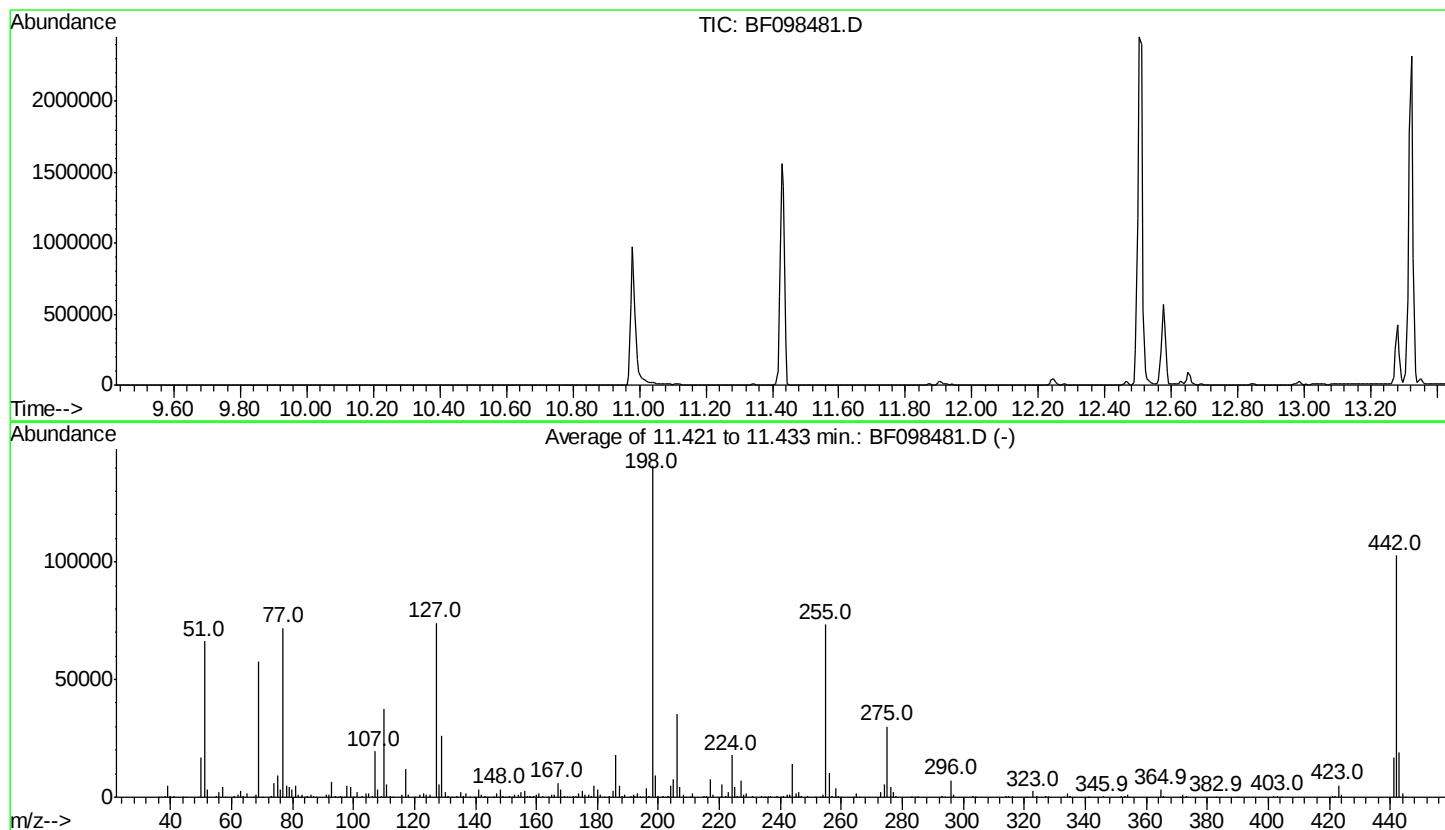

AutoFind: Scans 1587, 1588, 1589; Background Corrected with Scan 1582

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 47.0      | 66157   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 1021    | PASS             |
| 69          | 198          | 0.00         | 100          | 40.8      | 57520   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.5       | 261     | PASS             |
| 127         | 198          | 10           | 80           | 52.5      | 74008   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.2       | 329     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 140877  | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 9301    | PASS             |
| 275         | 198          | 10           | 60           | 21.4      | 30094   | PASS             |
| 365         | 198          | 1            | 100          | 2.2       | 3166    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.5      | 16933   | PASS             |
| 442         | 198          | 50           | 100          | 72.9      | 102650  | PASS             |
| 443         | 442          | 15           | 24           | 18.4      | 18861   | PASS             |